




Scene 1: Bed empty




Scene 1: Bed empty (suboptimal recording)




Scene 2: Subject in bed, wires being attached for standard monitoring




Scene 3: Subject in bed detaches wires

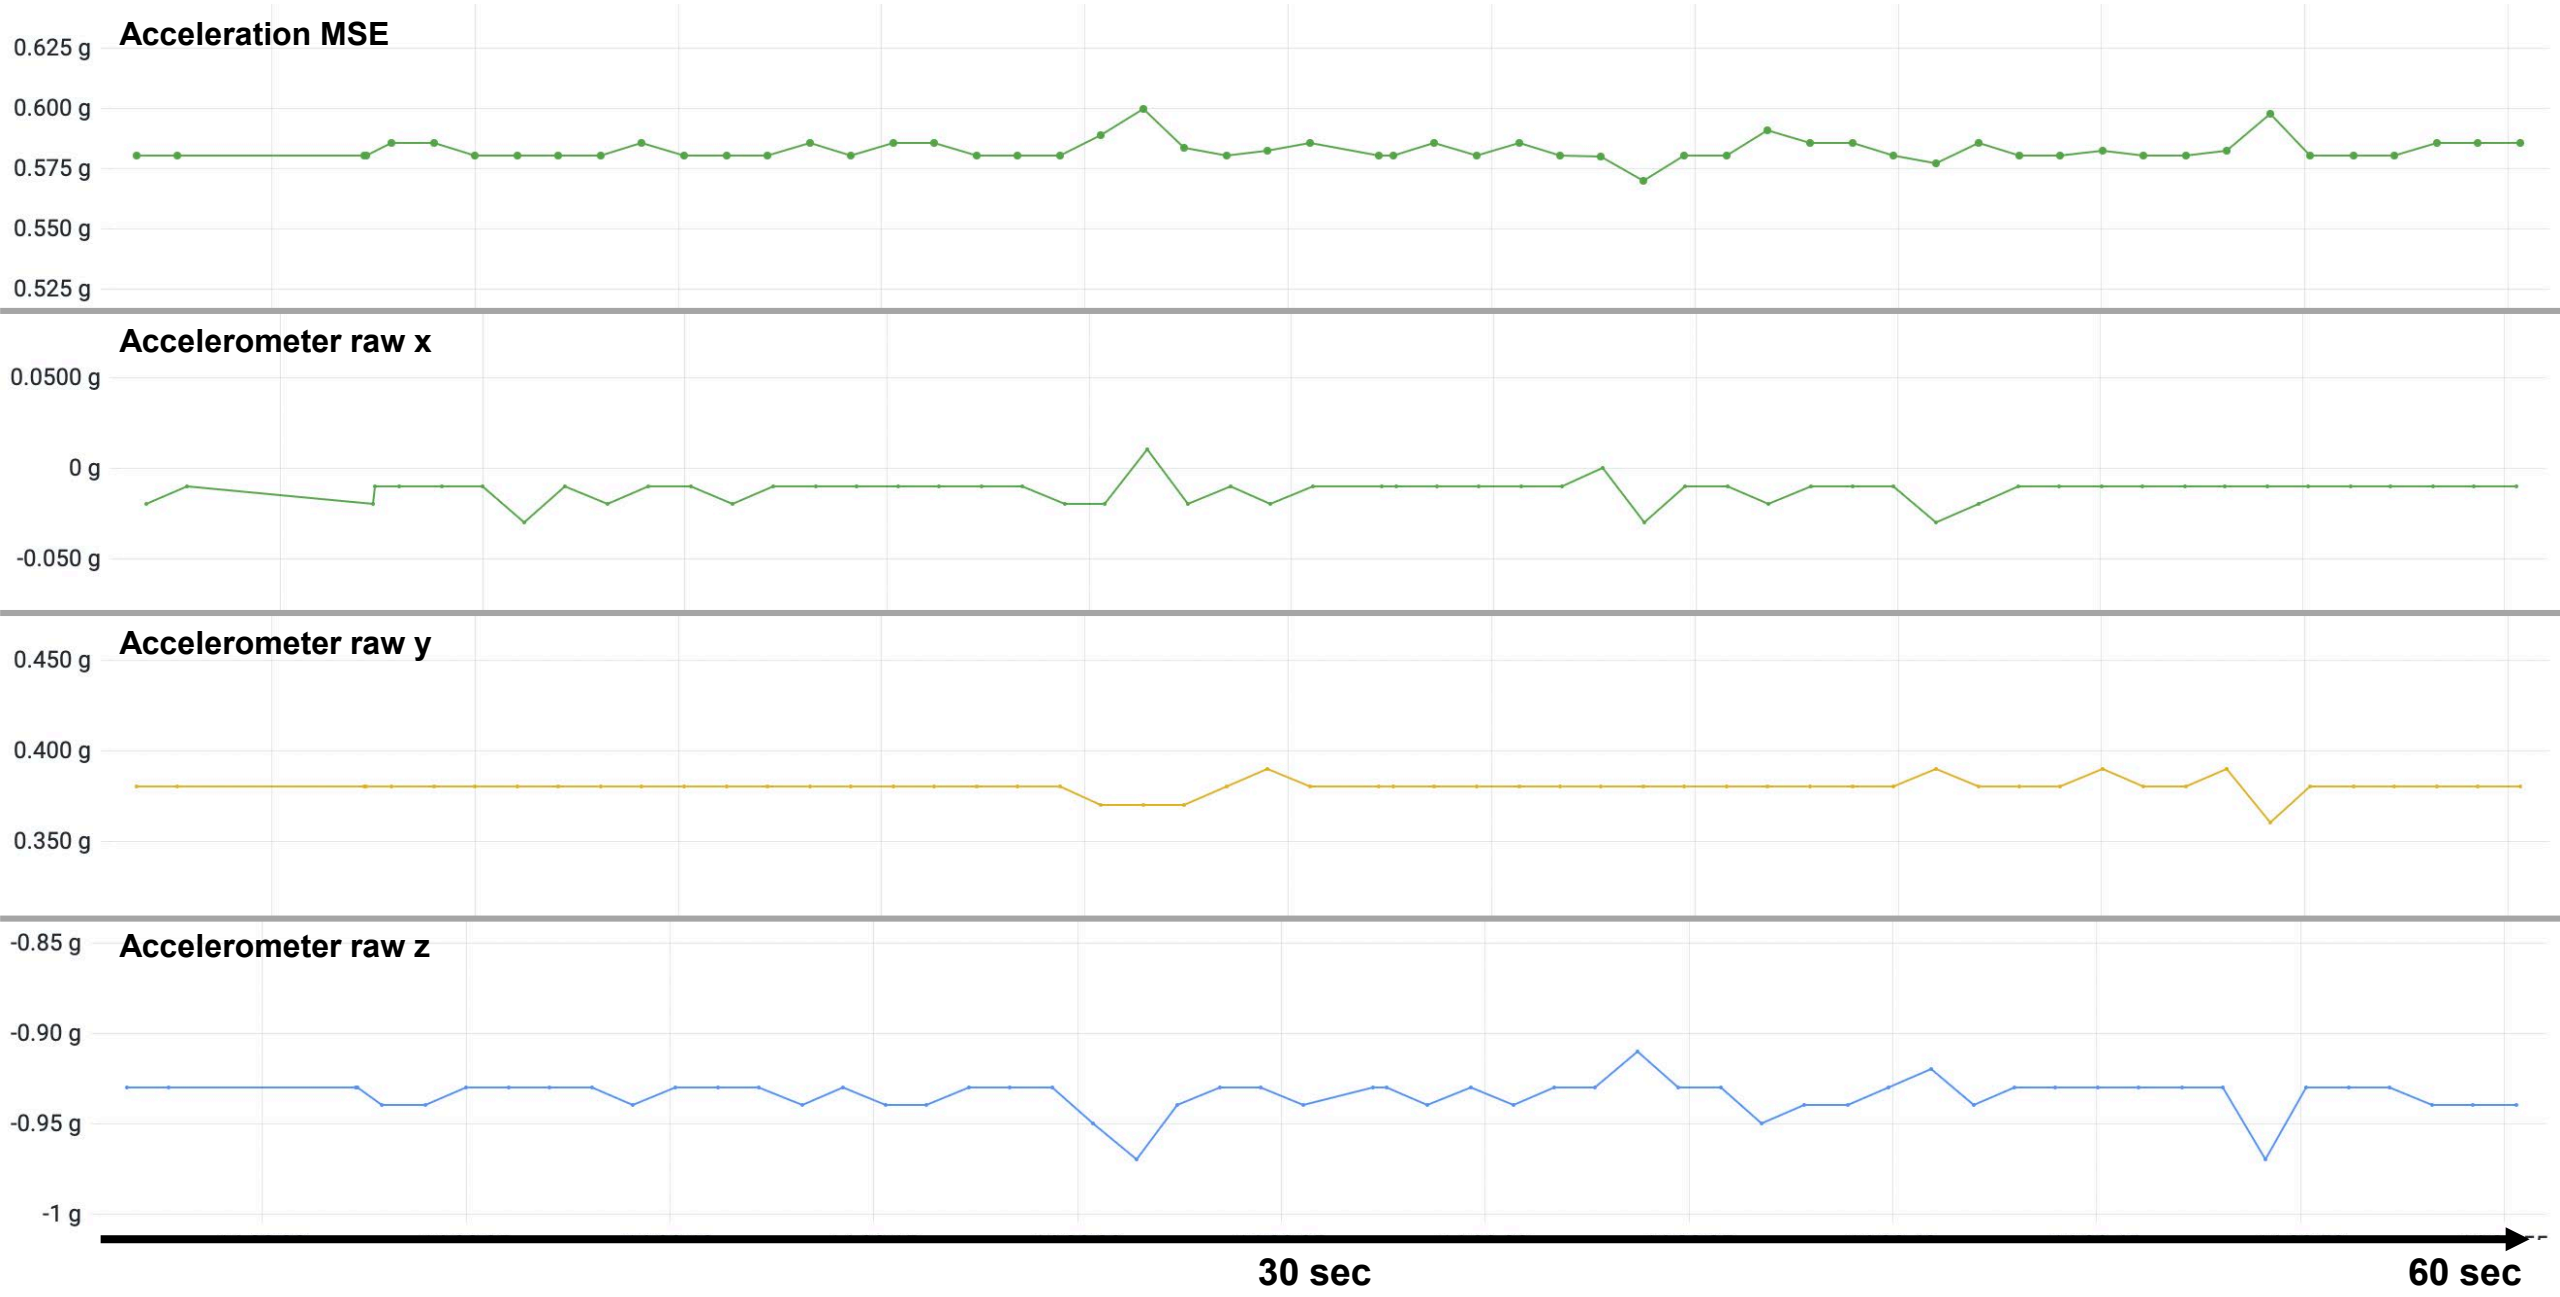


Scene 4: Subject in bed, lying uneasy and restless

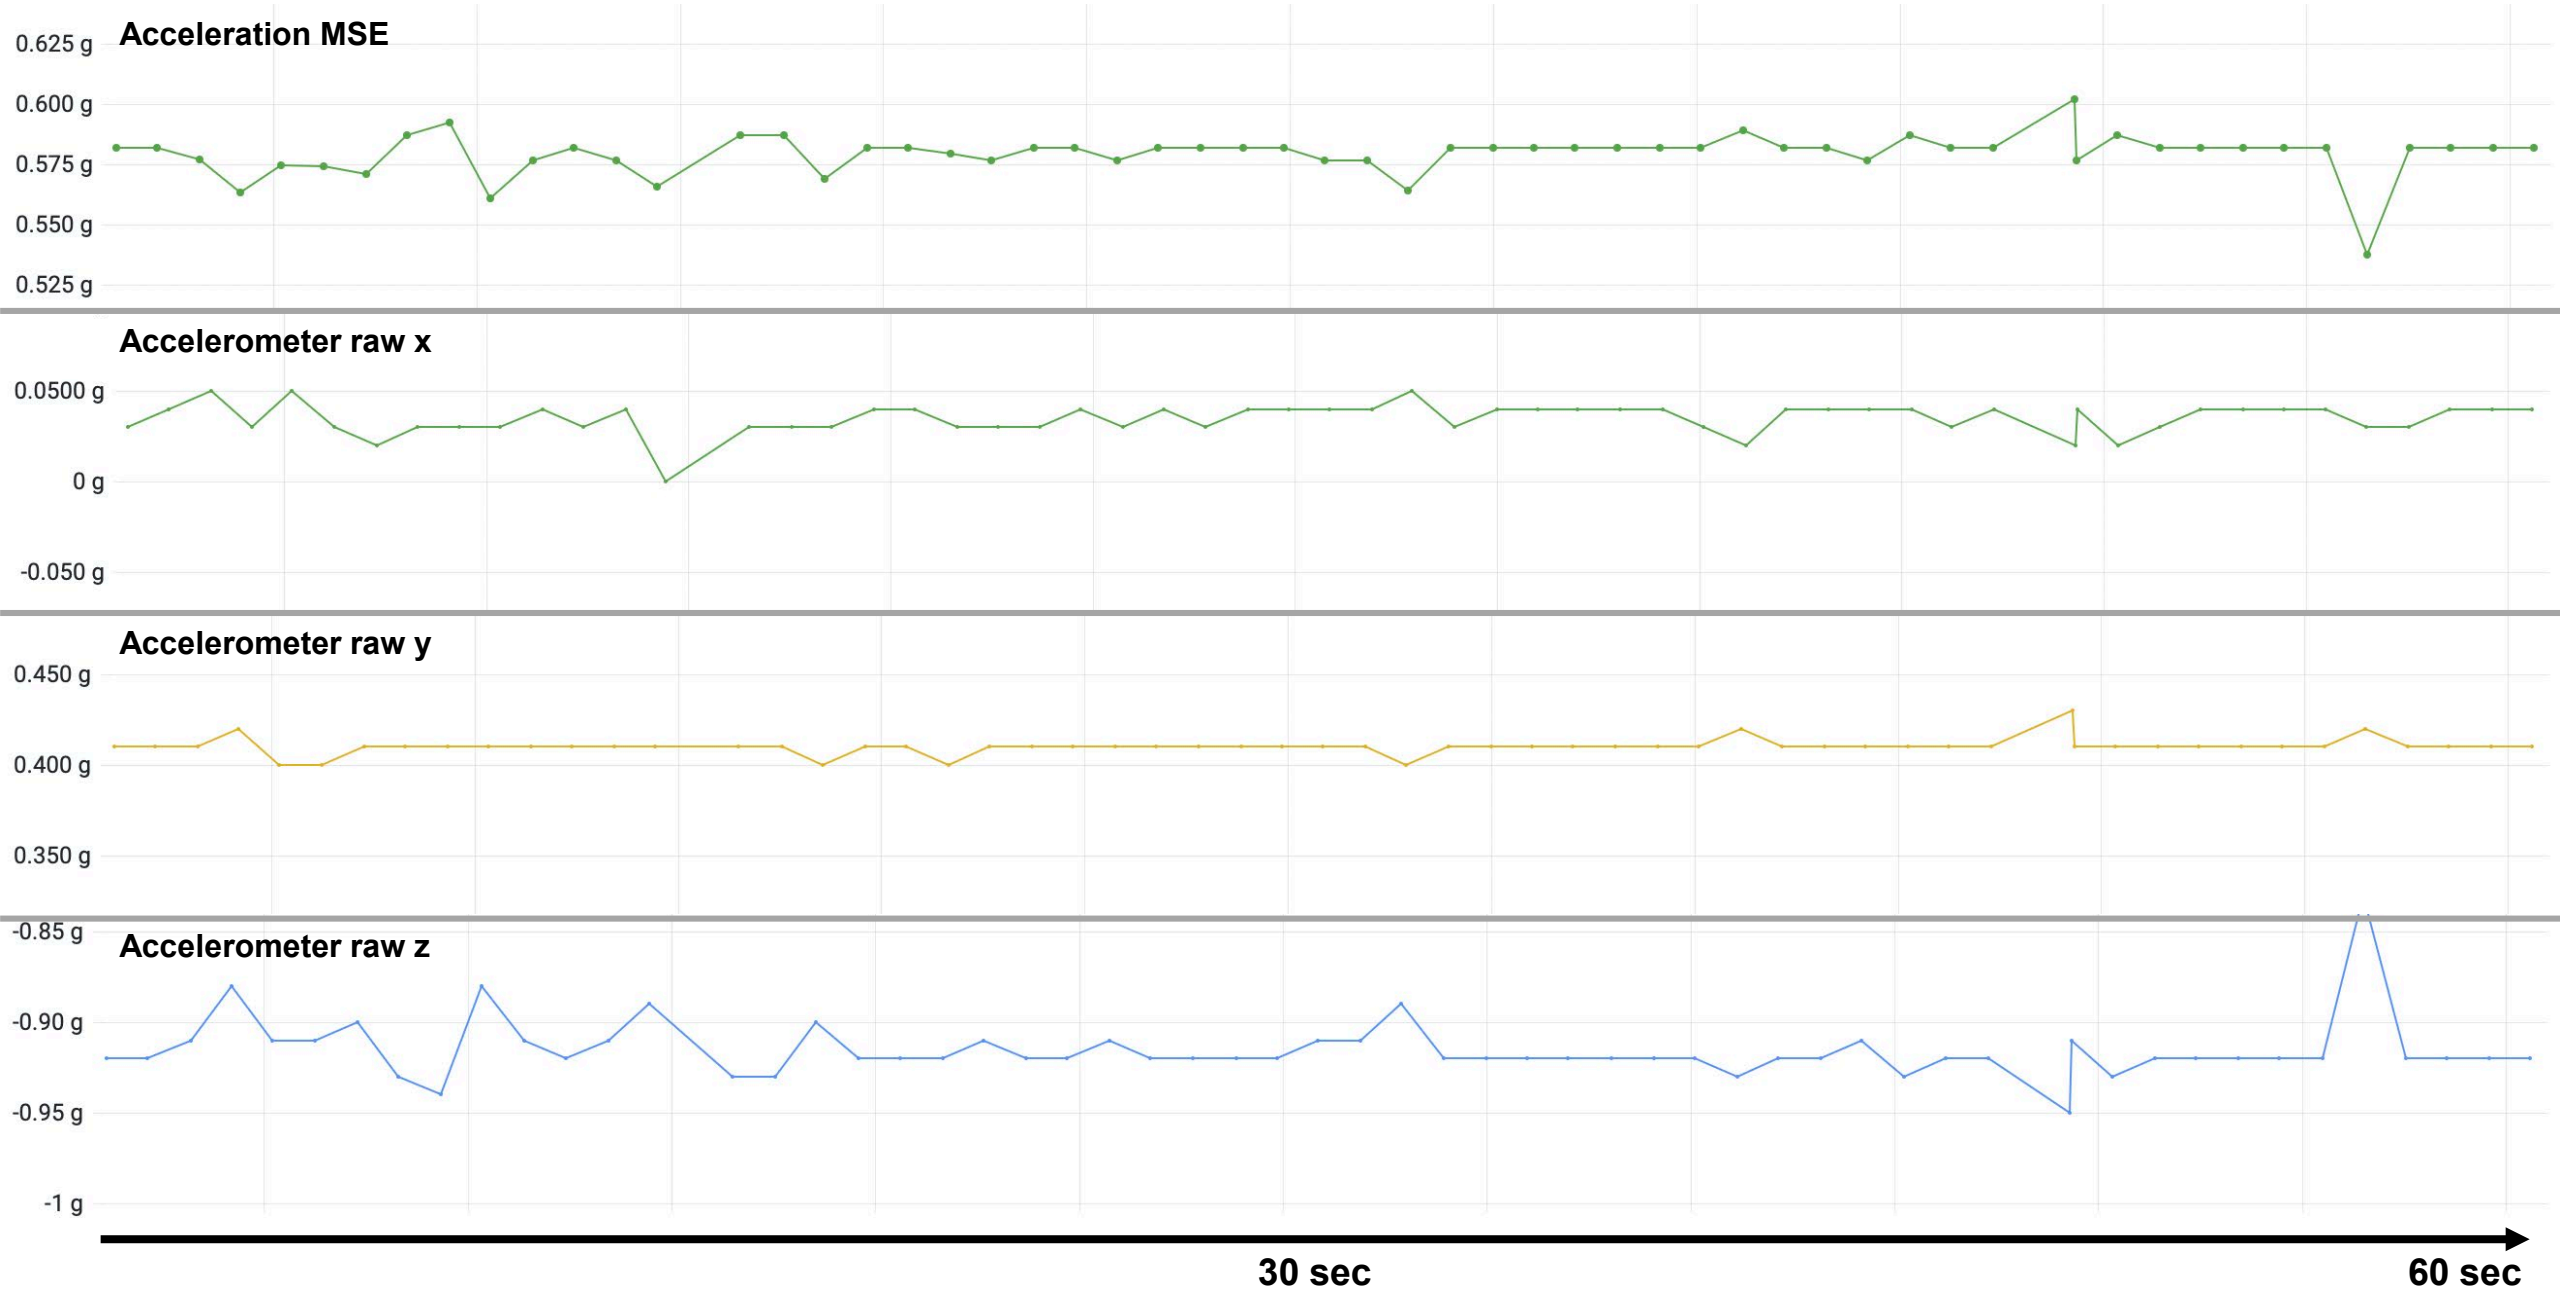


Scene 5, 9, 12, 15, 17: Subject lying in bed motionless, breathing shallow

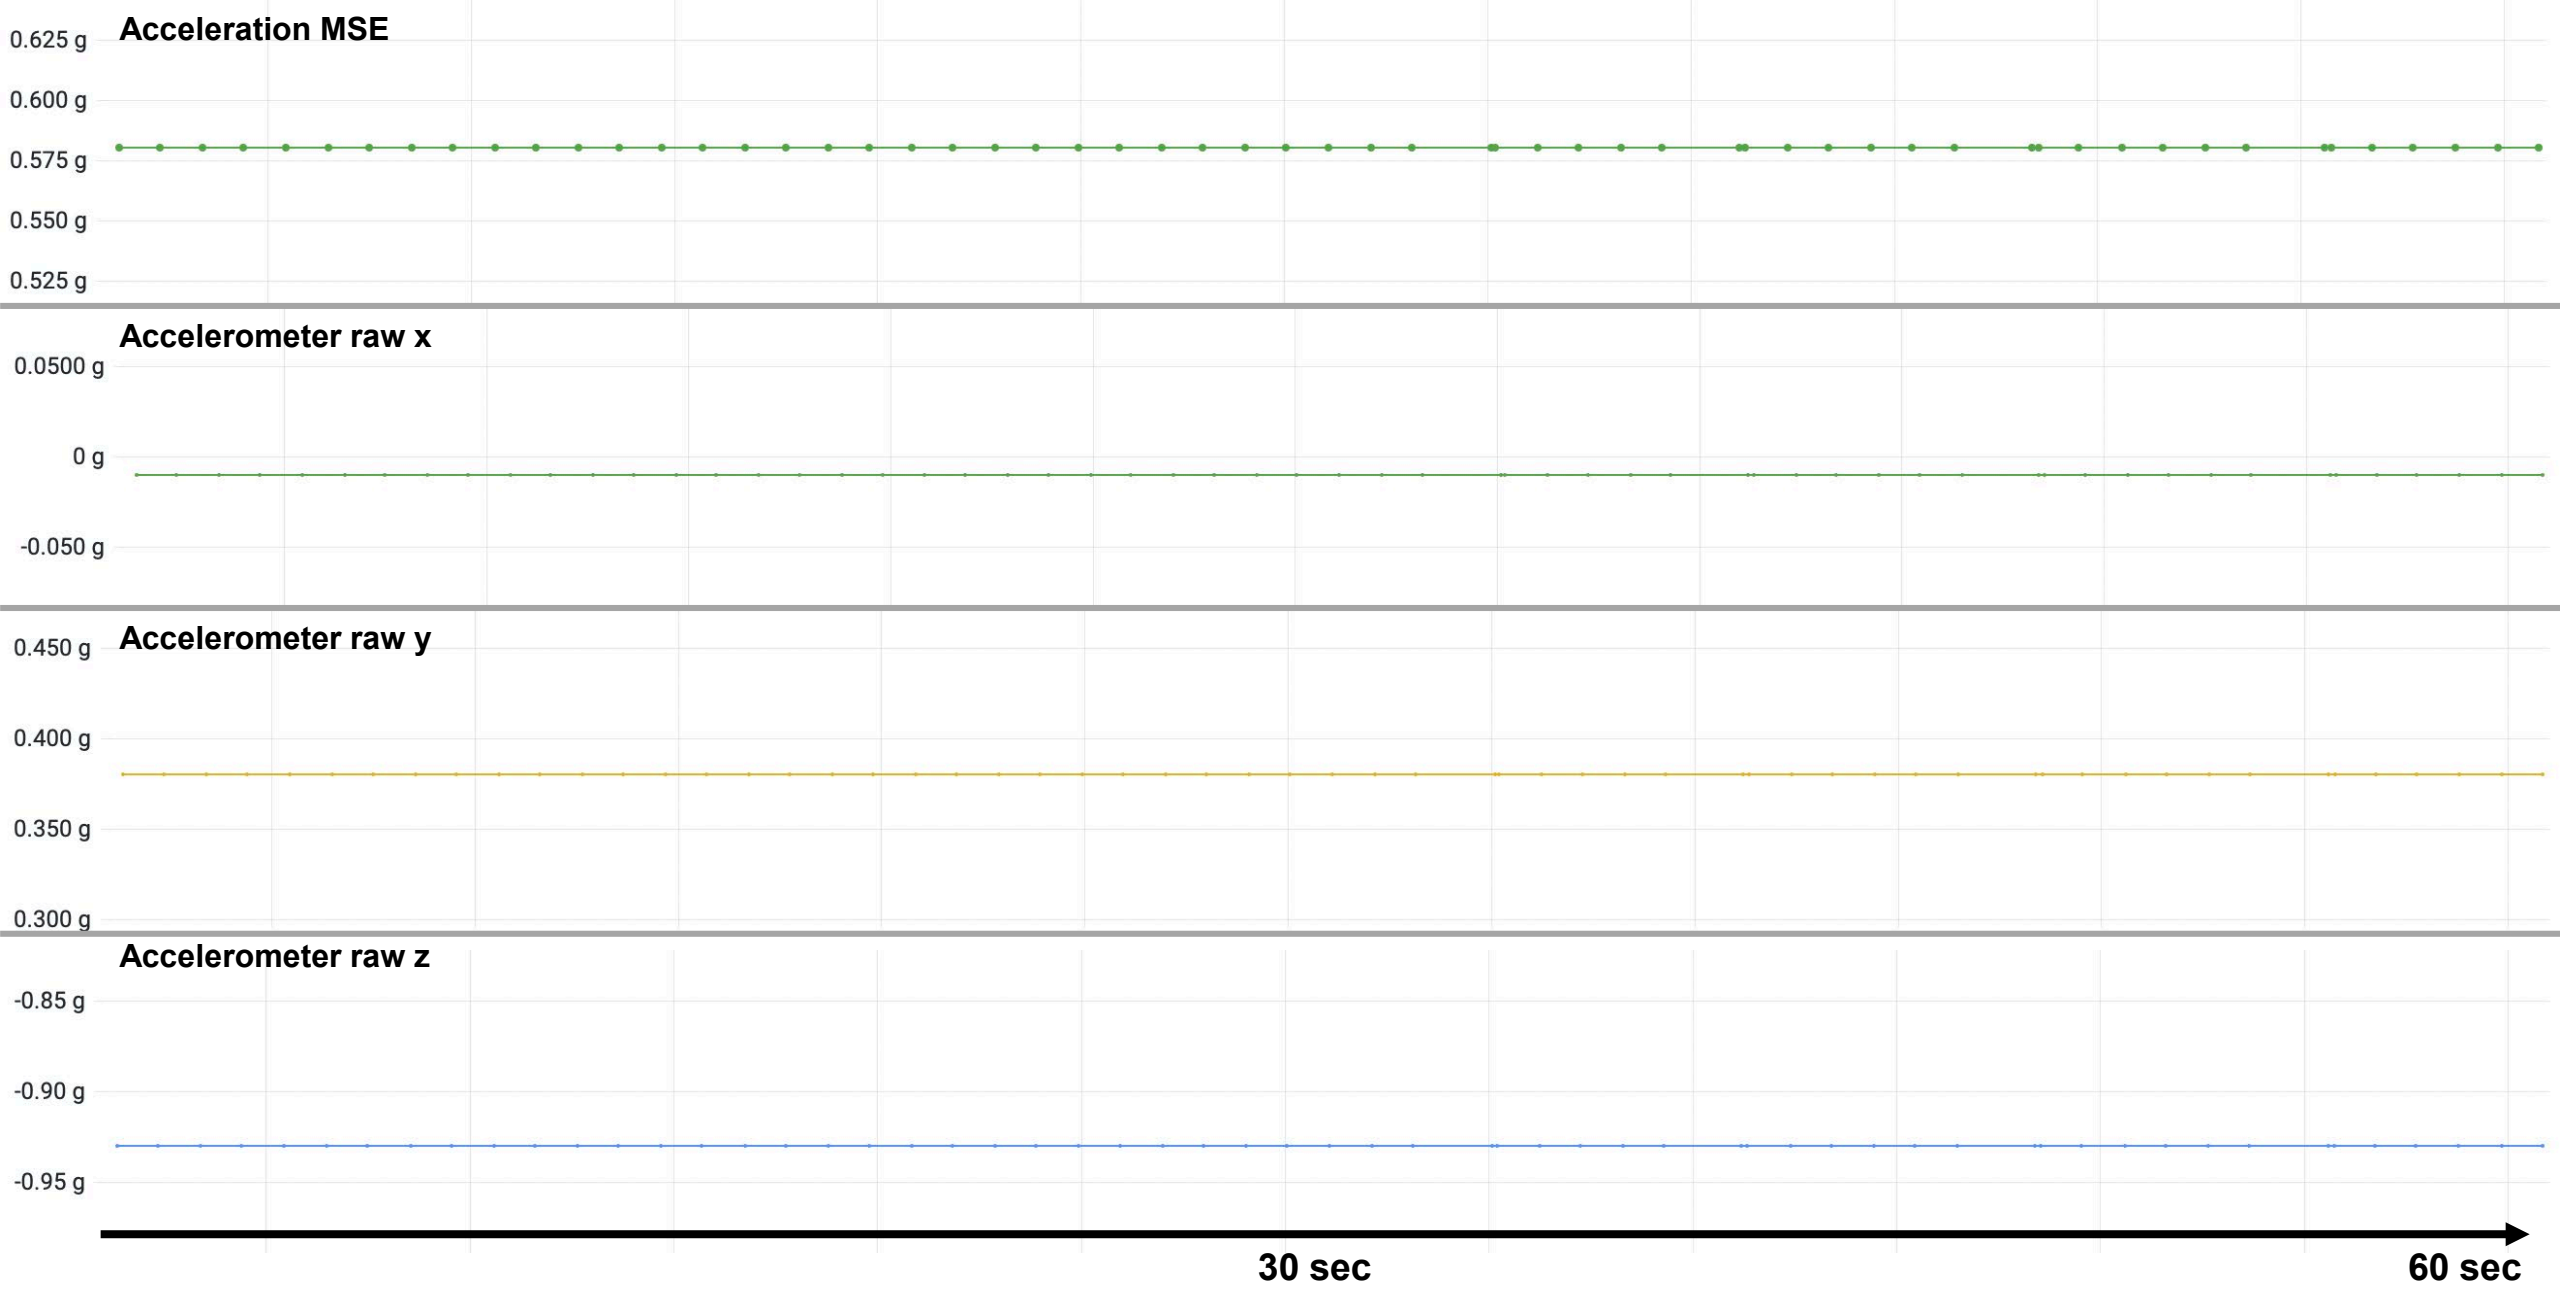


Scene 6: Subject in bed, tossing and turning

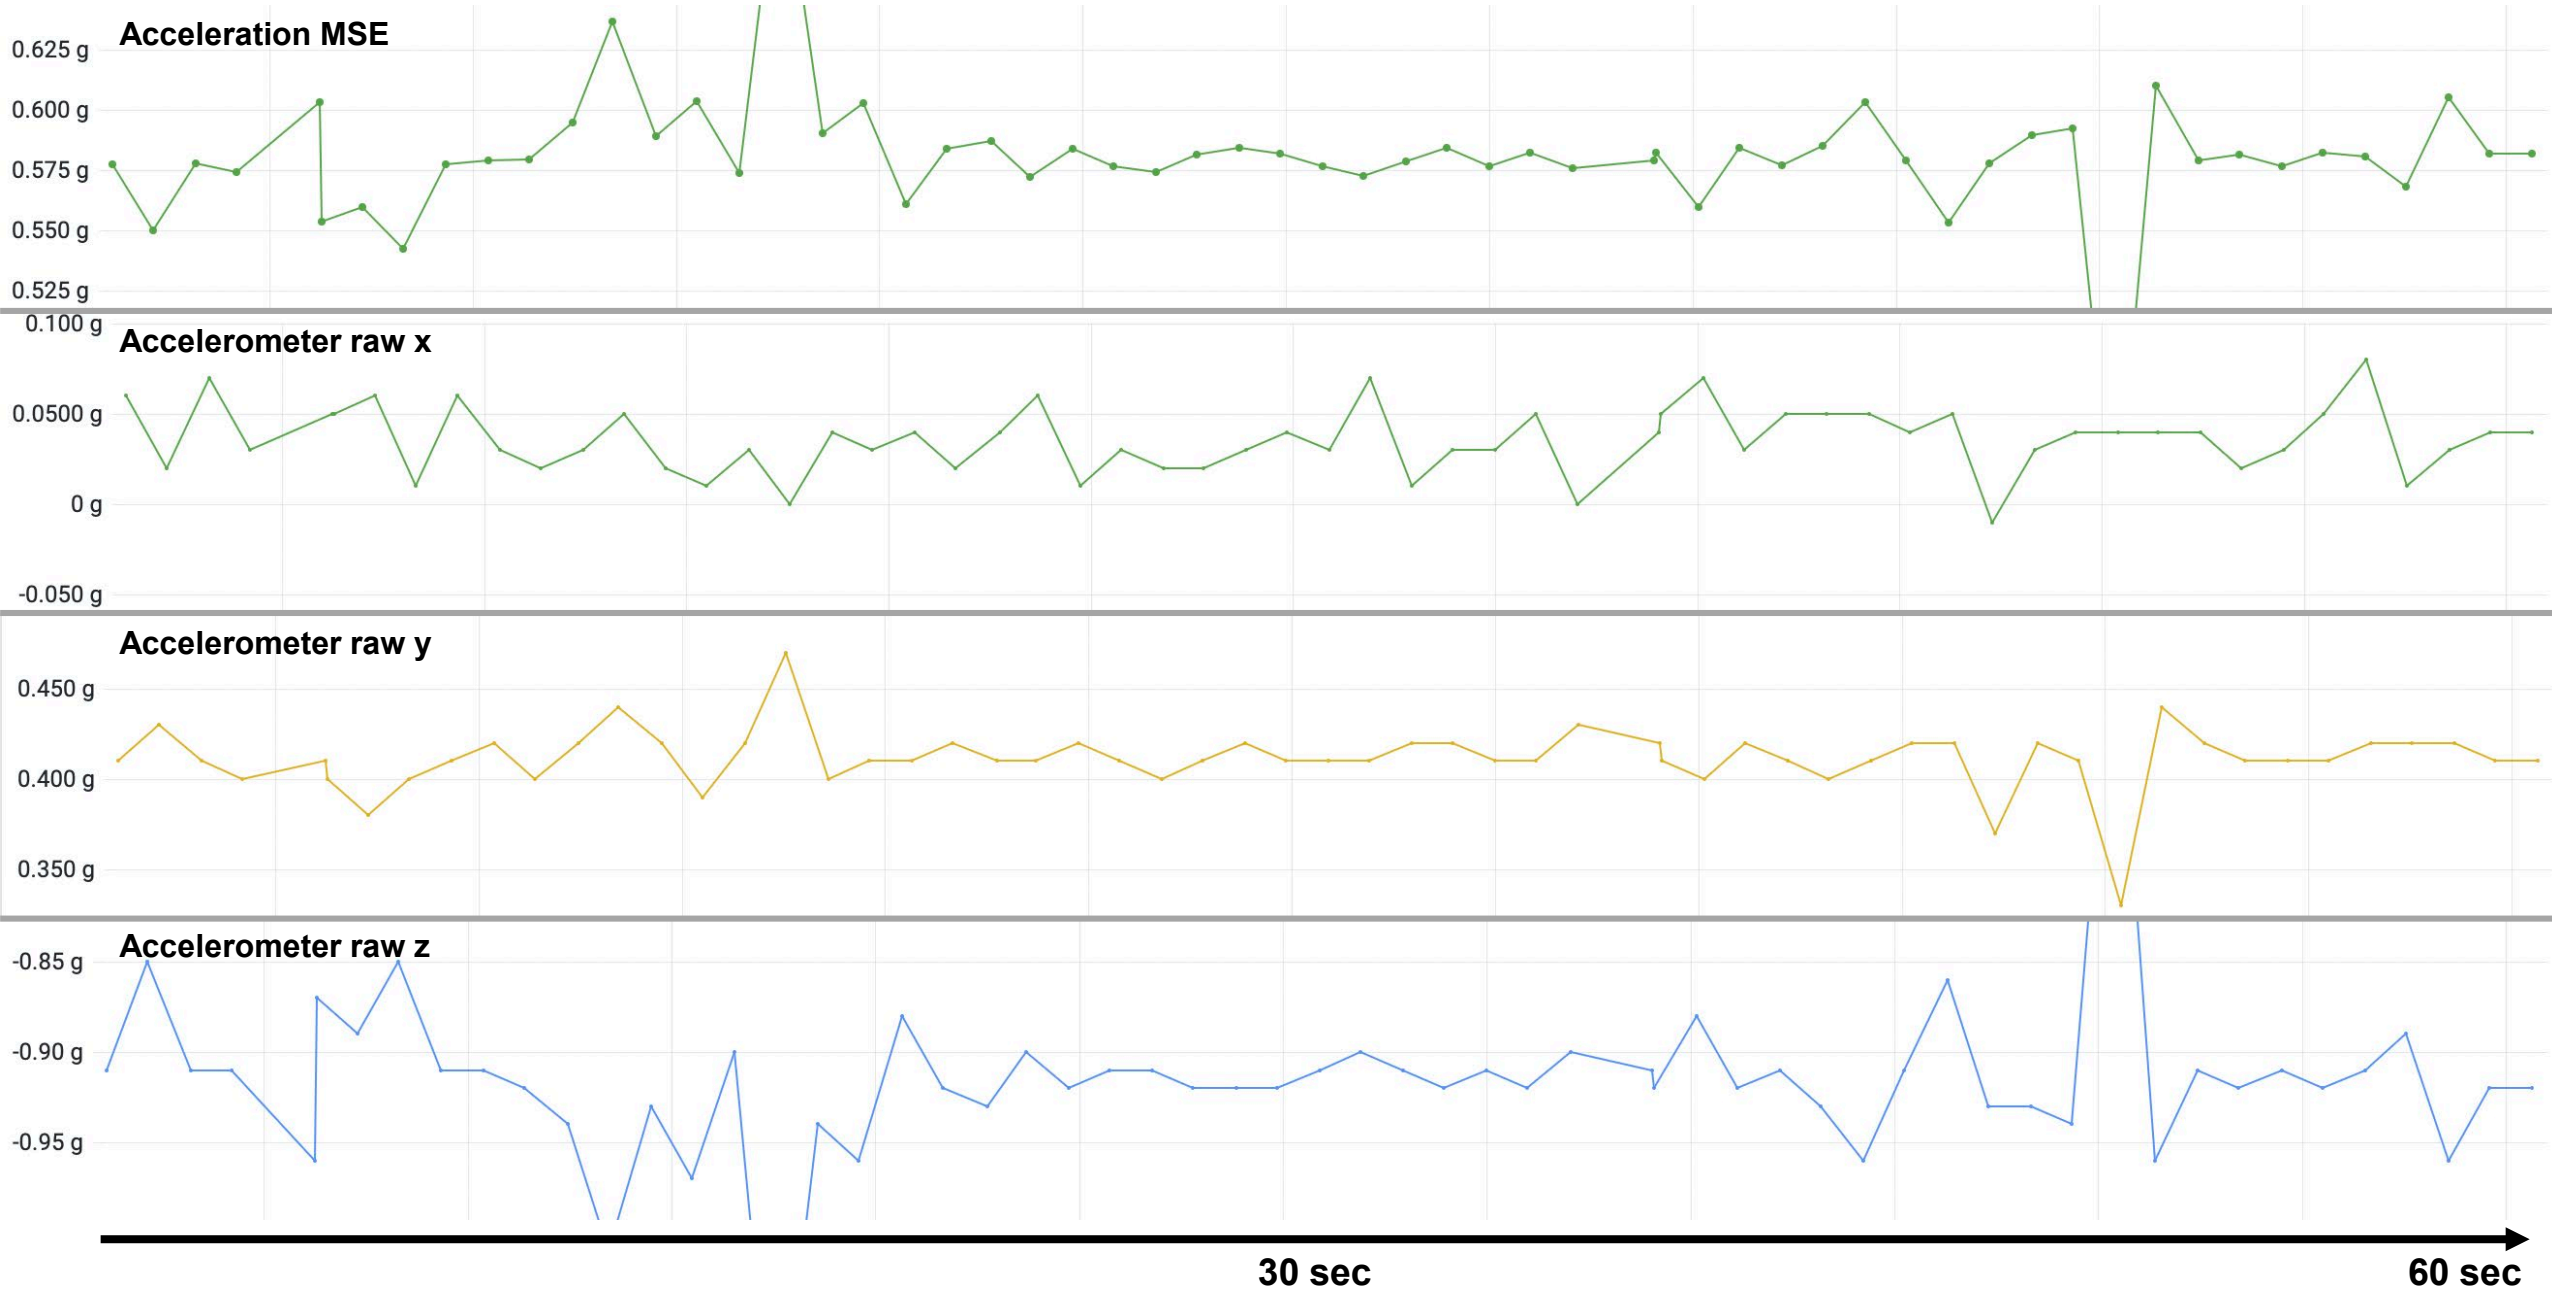


Scene 7: Subject lying in bed motionless, breathing normal

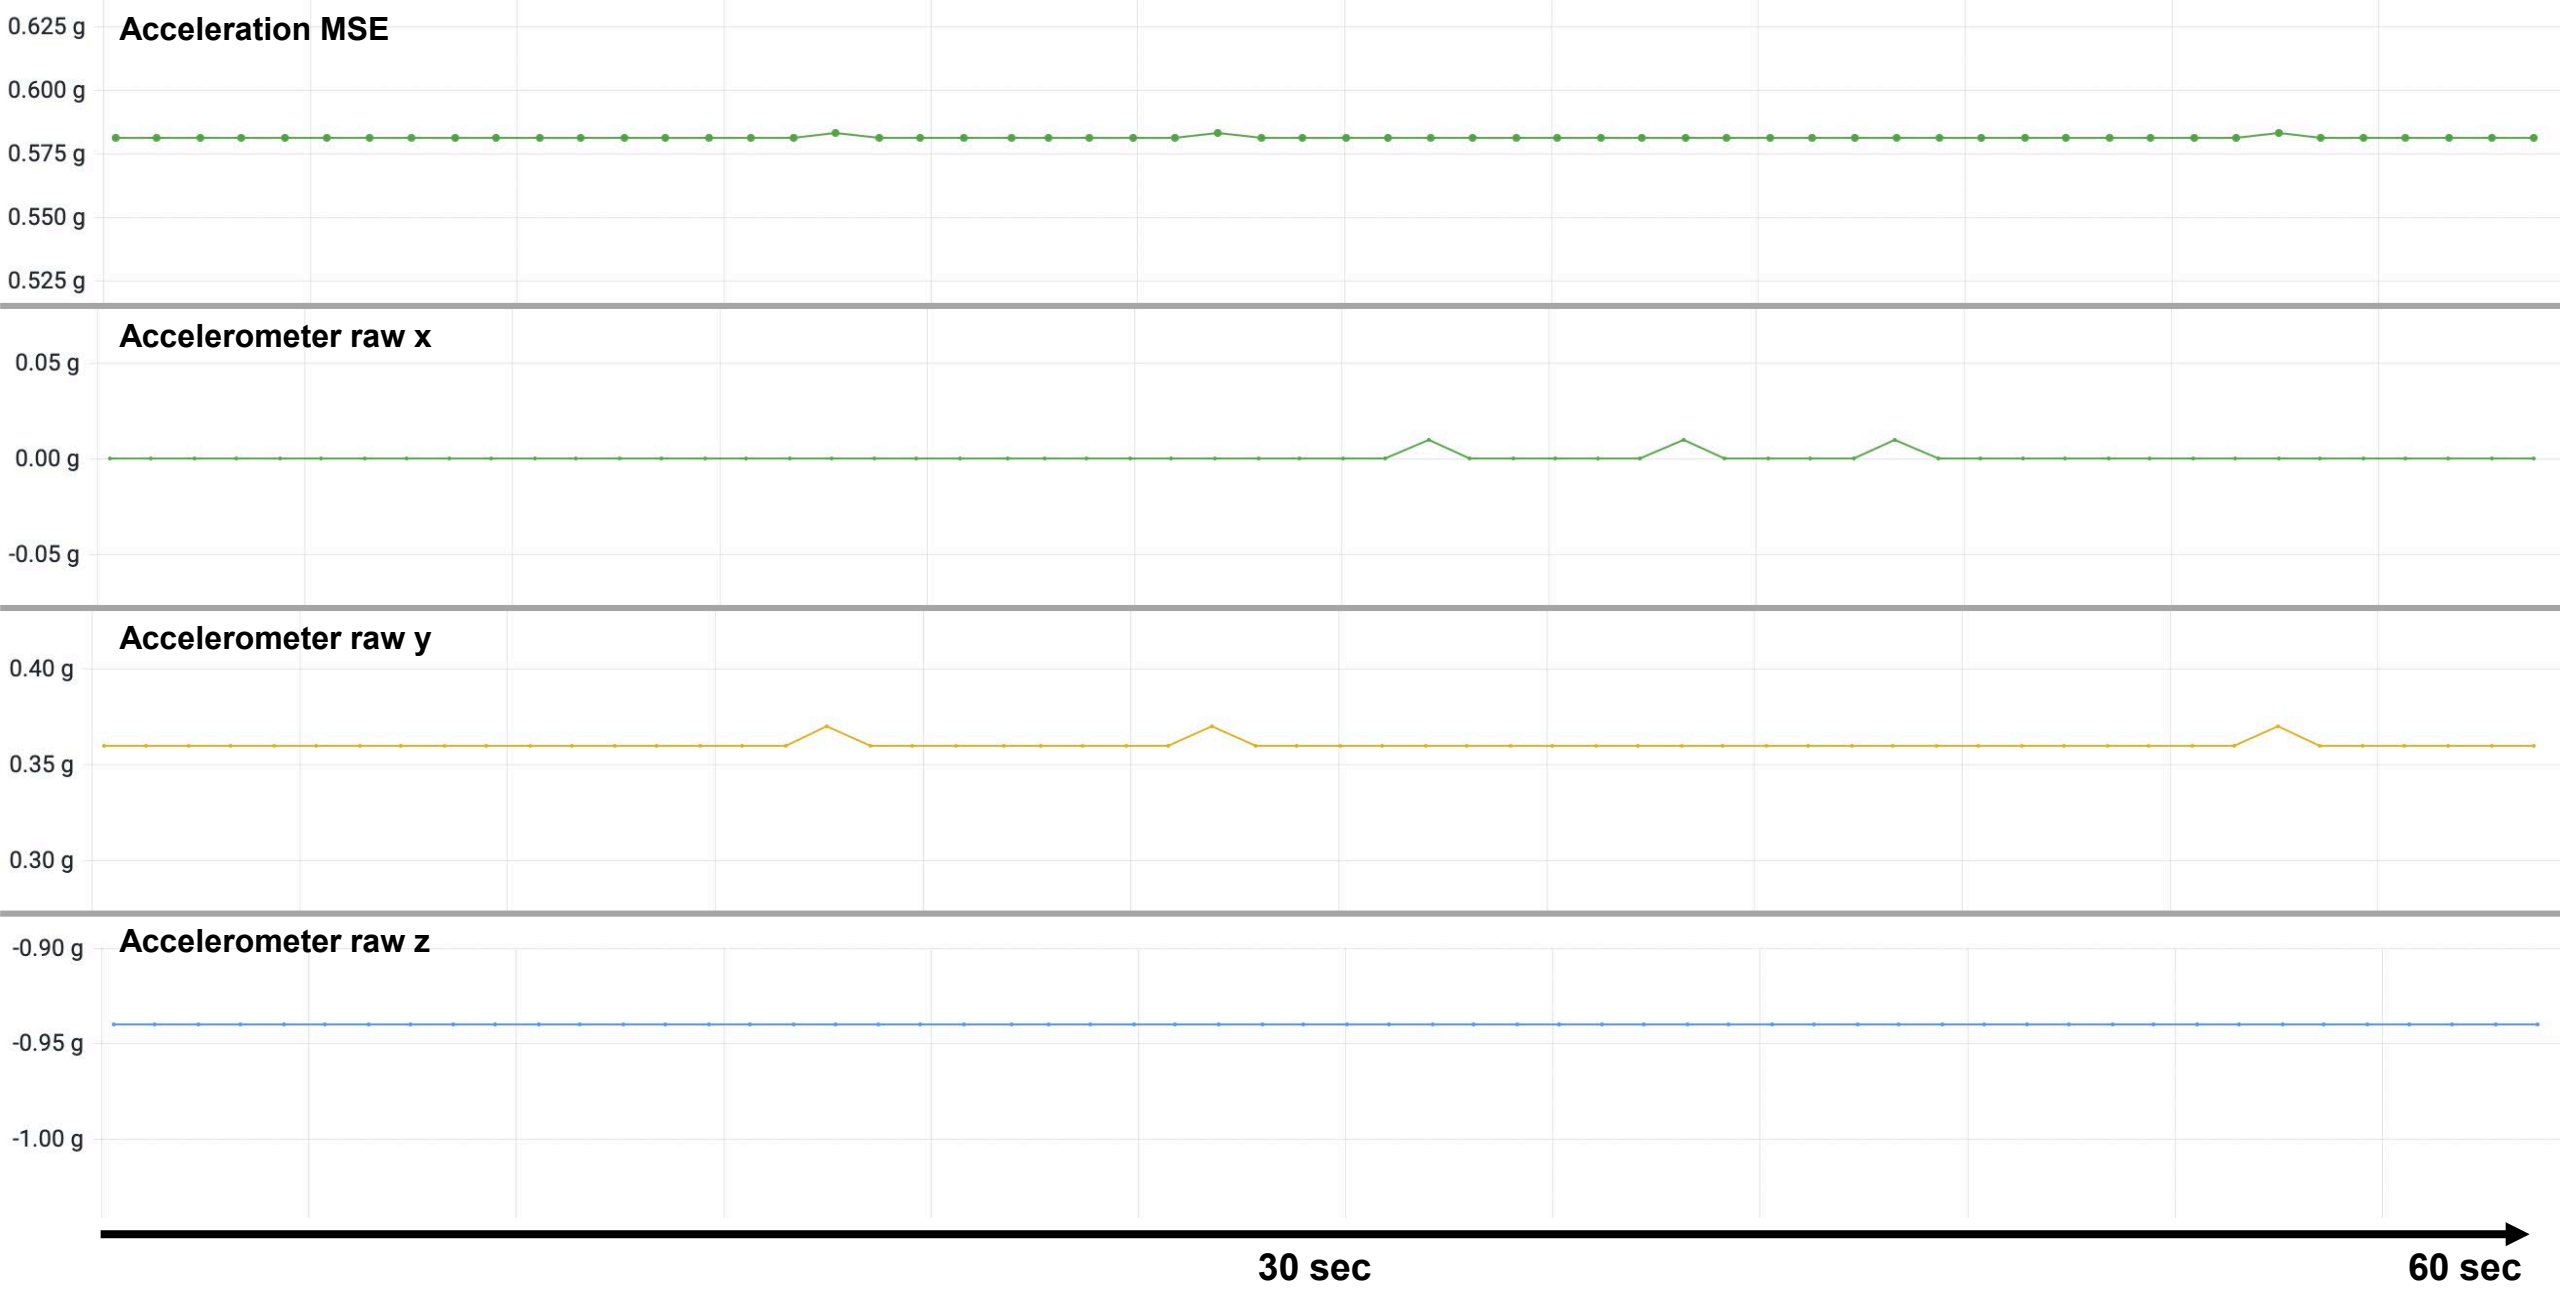


Scene 8: Subject in bed, jumping up and down

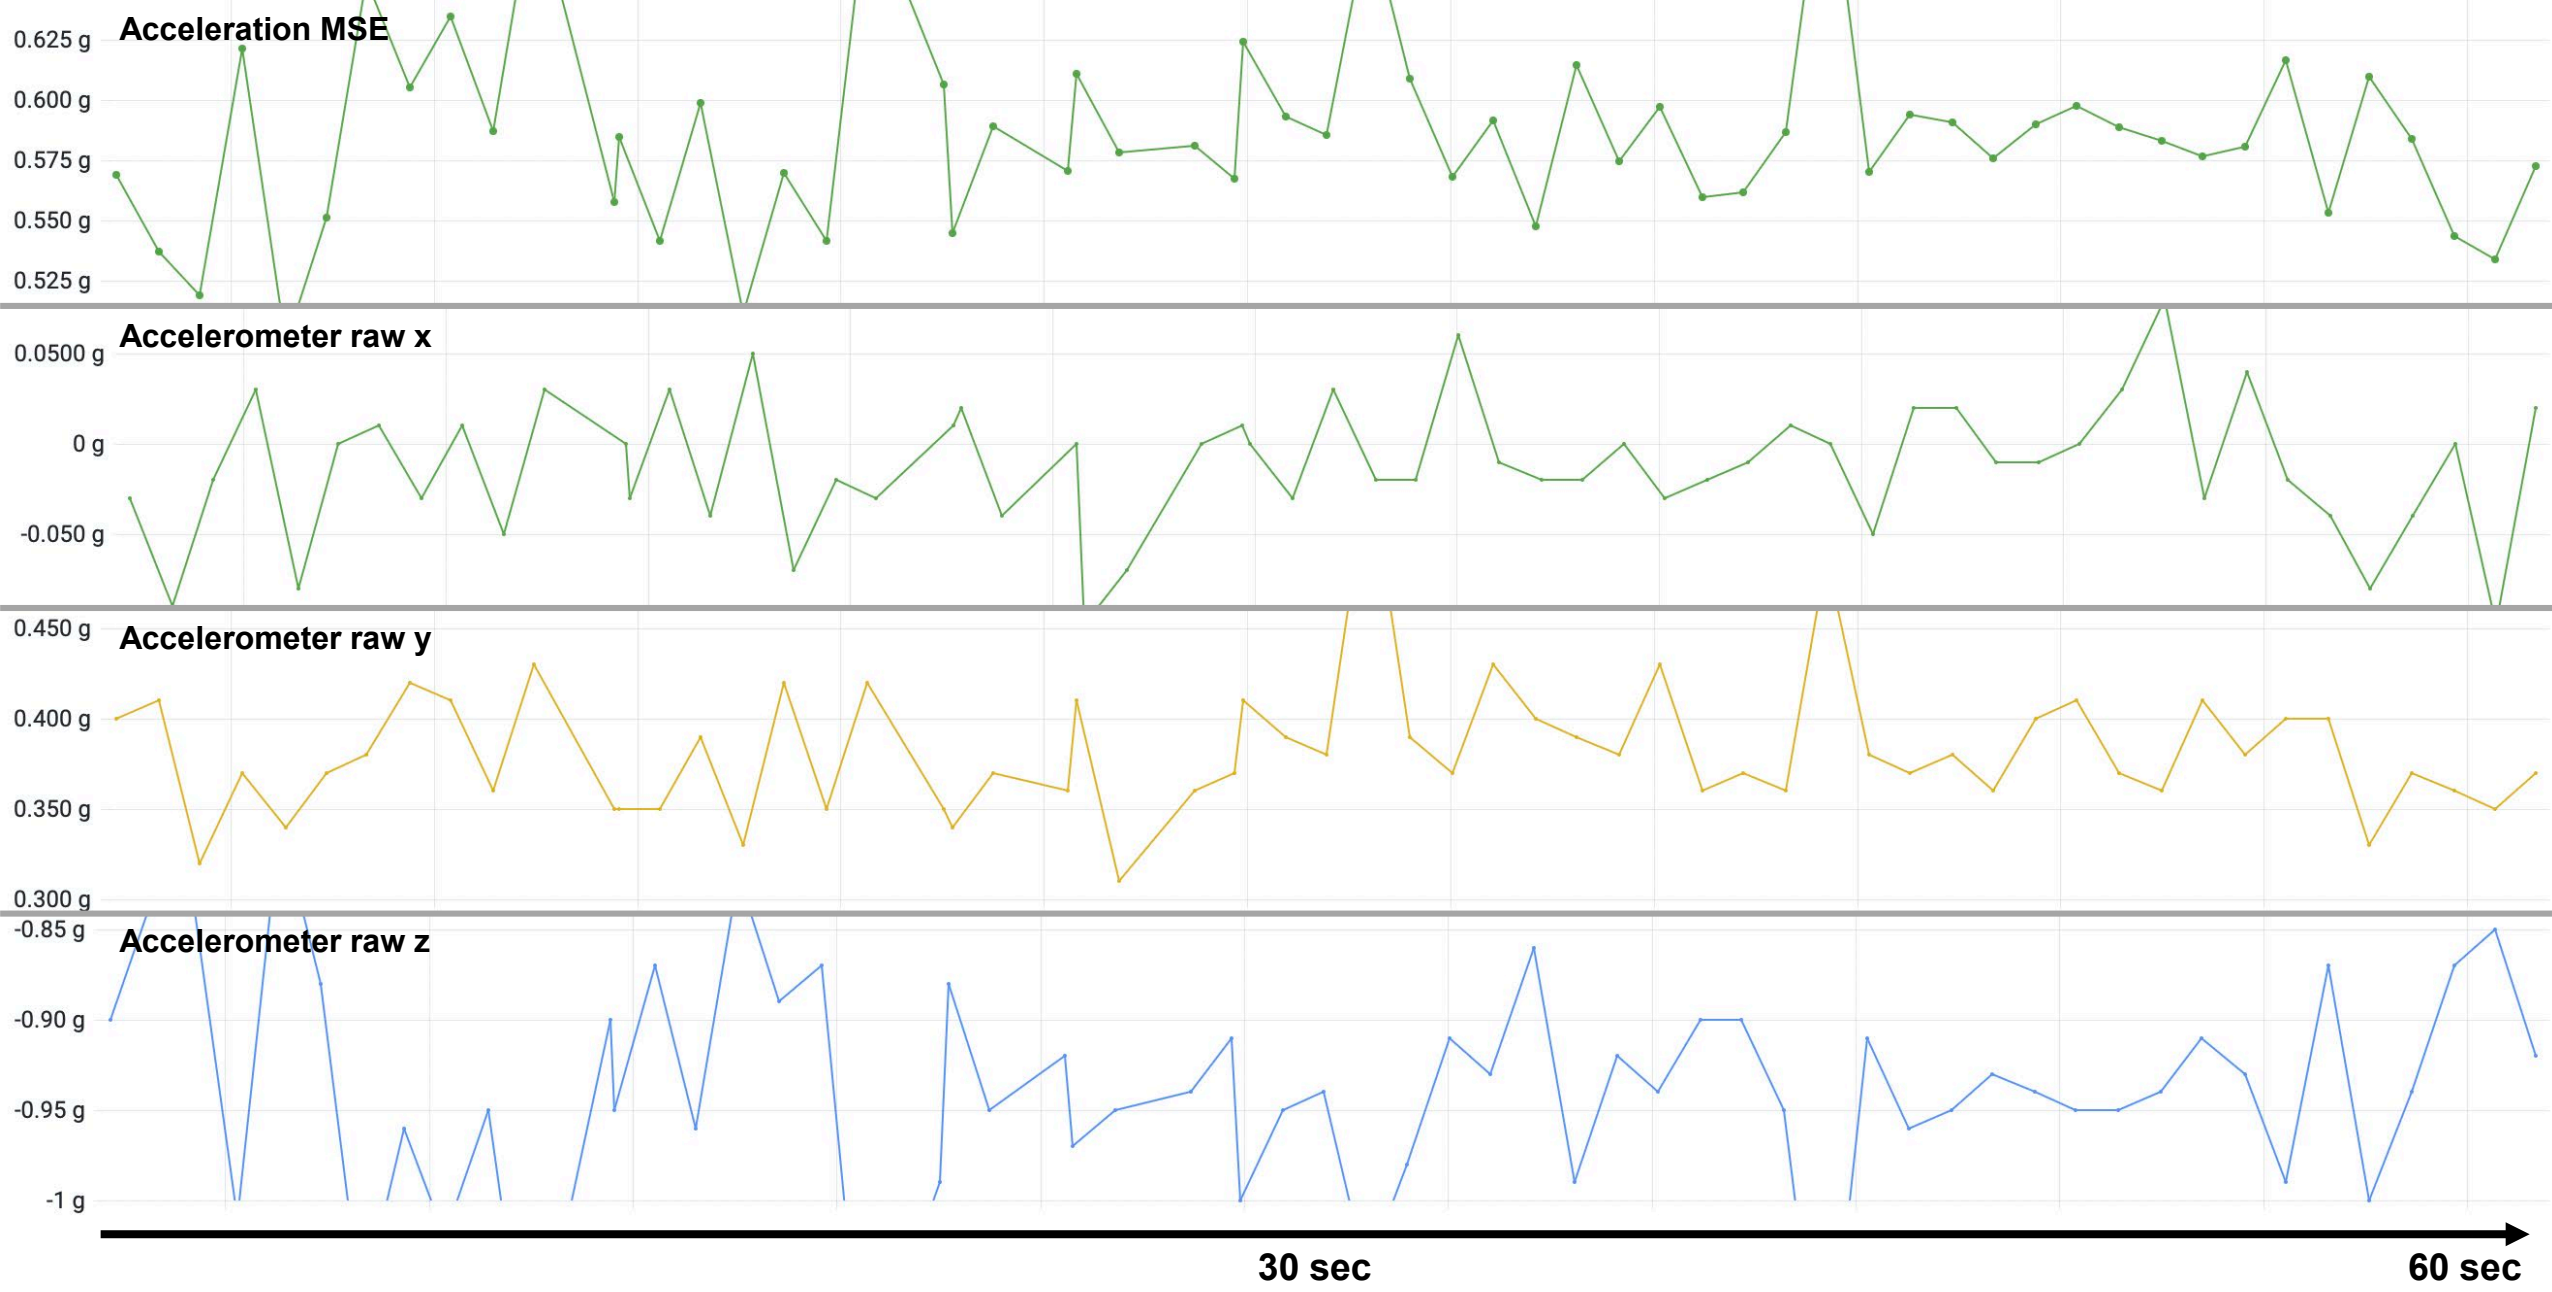


Scene 10: Subject in bed with little and careful movements

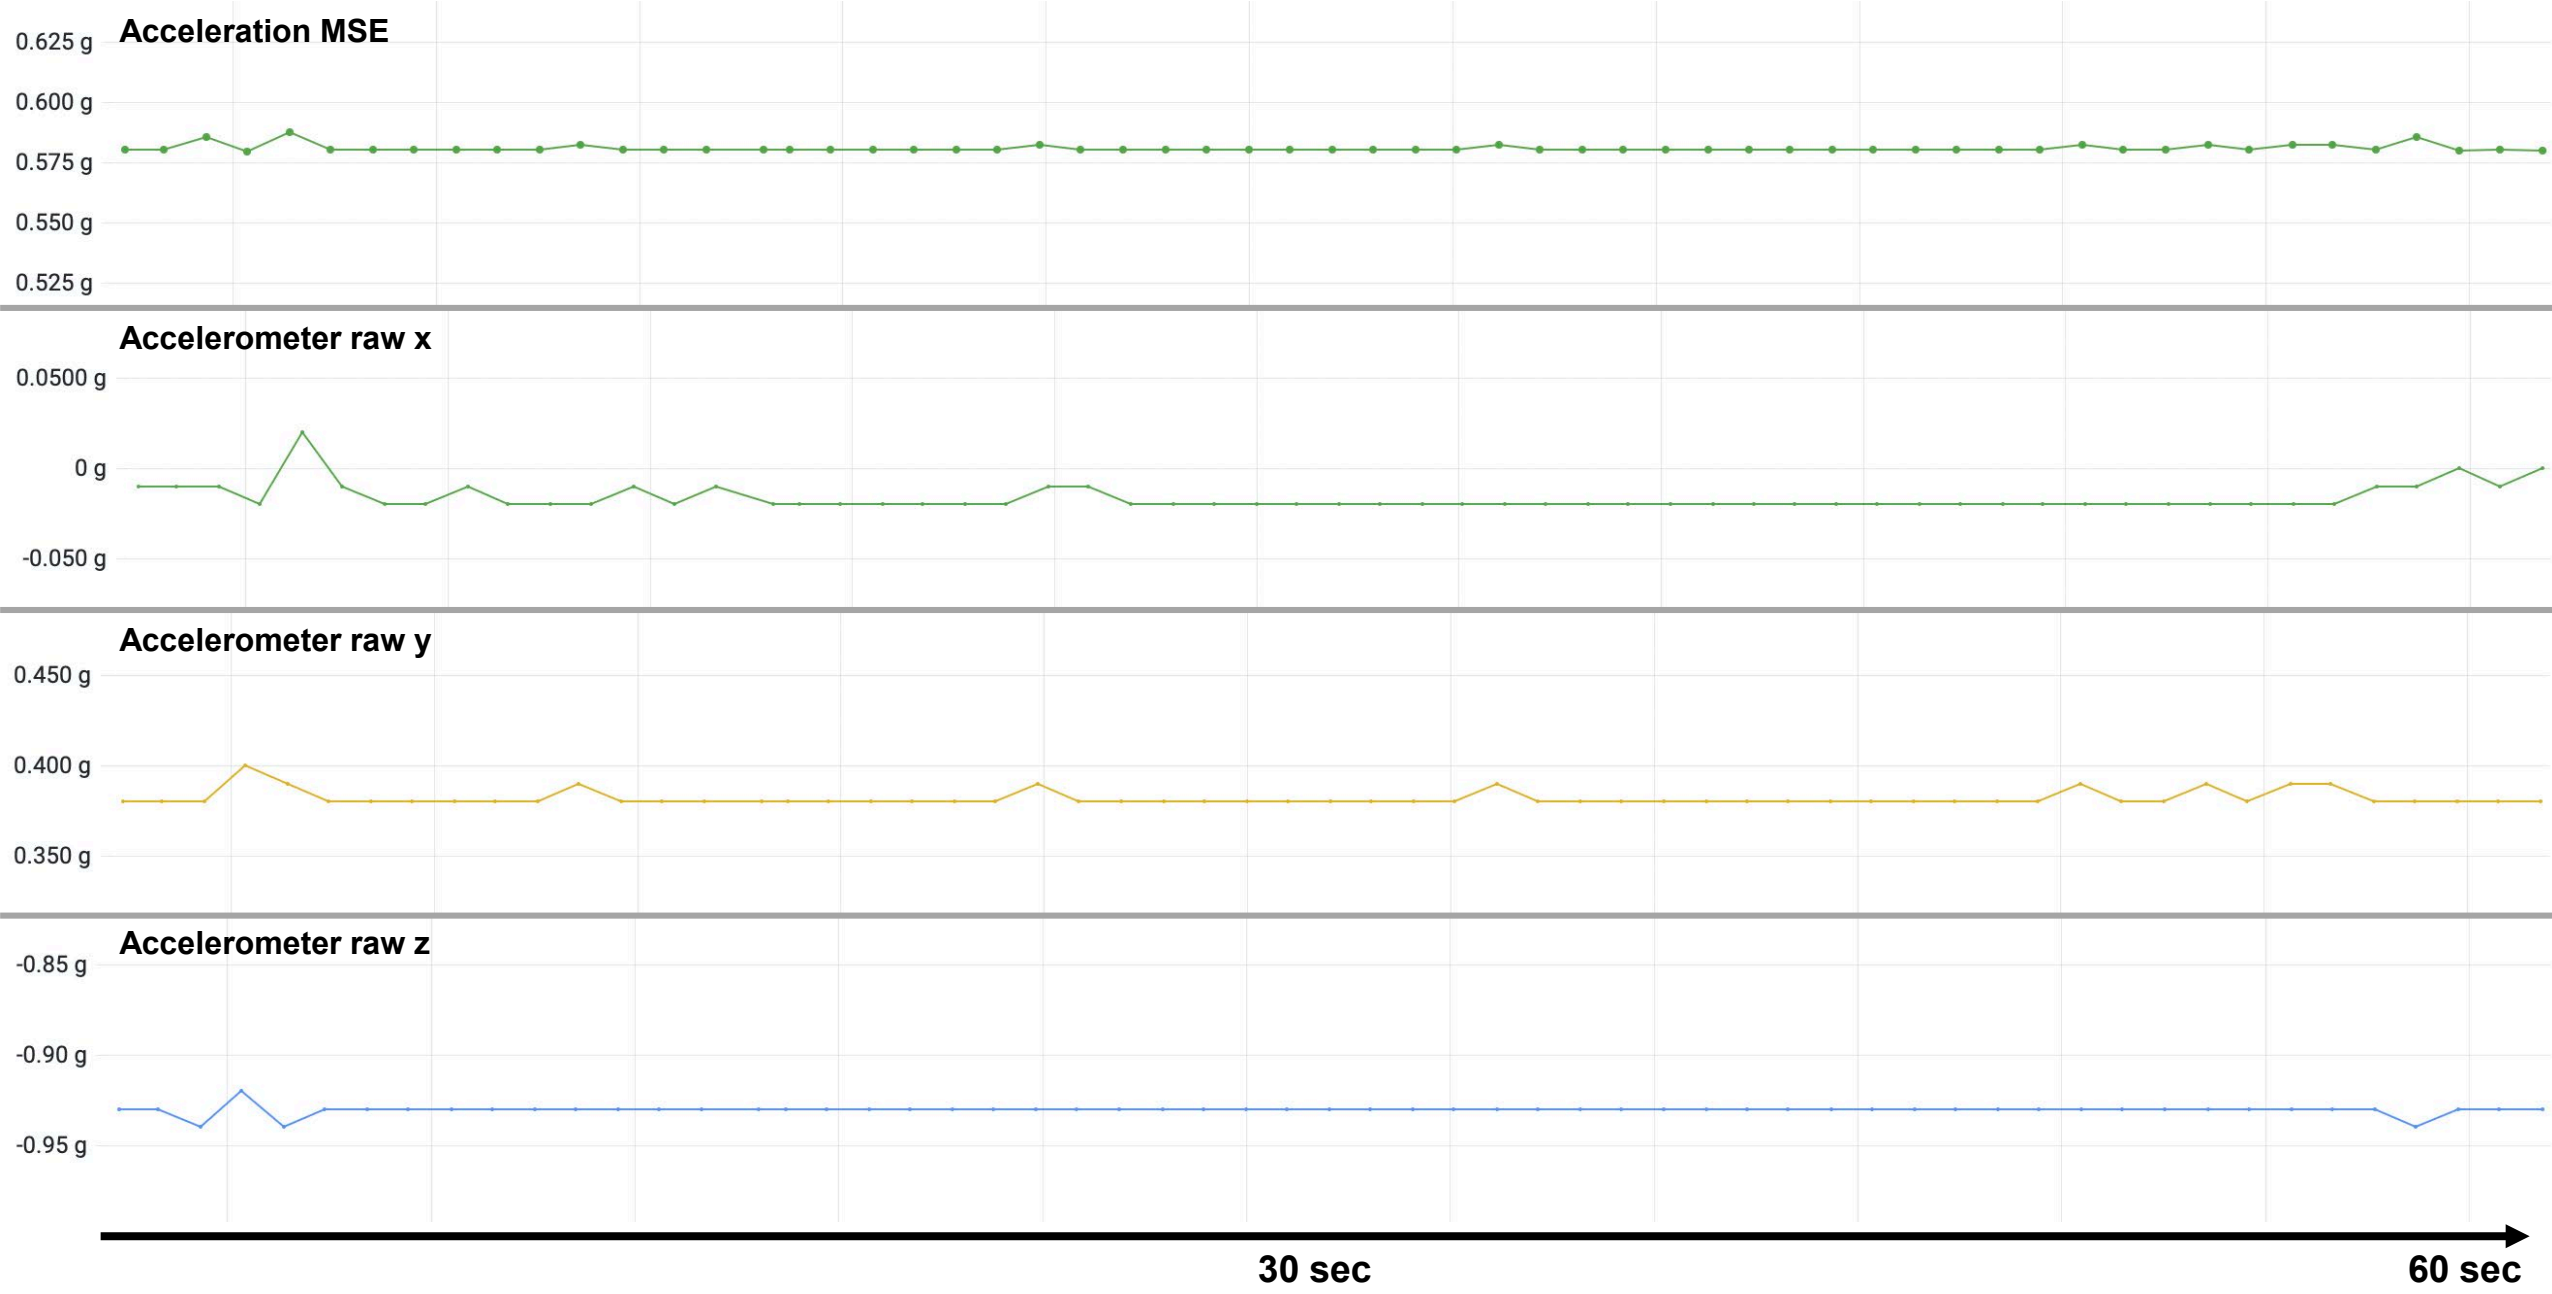


Scene 11: Subjects lying in bed motionless, breathing strong

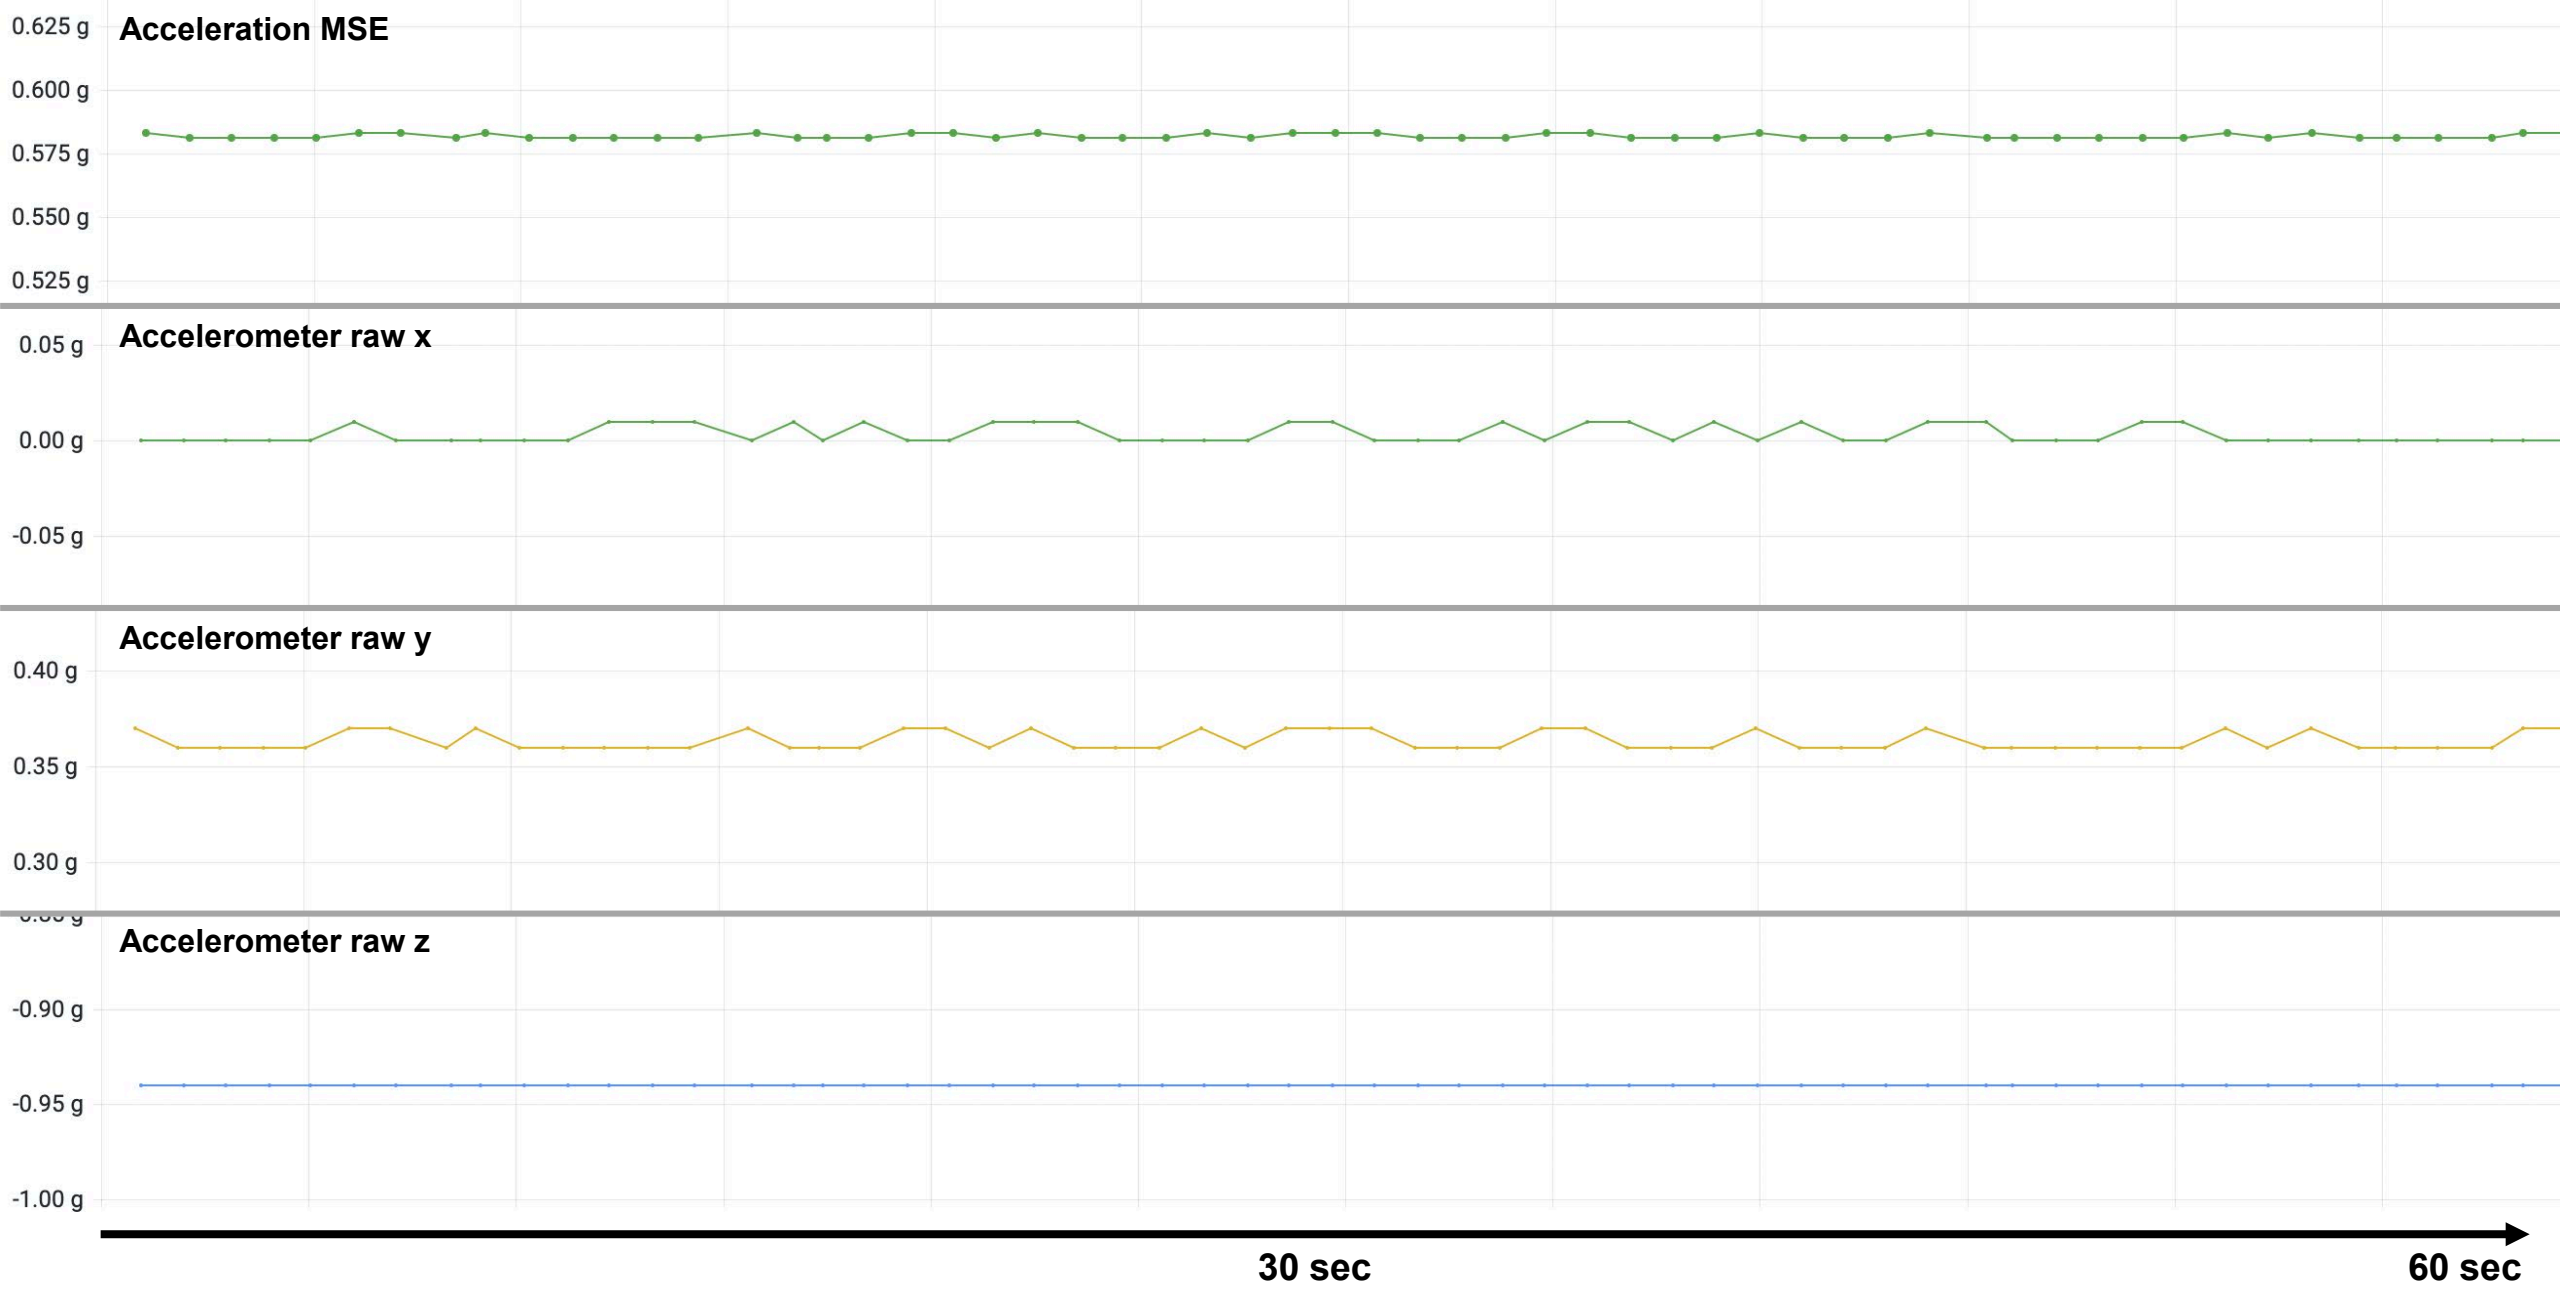


Scene 13: Subject in bed attempting to leave the bed

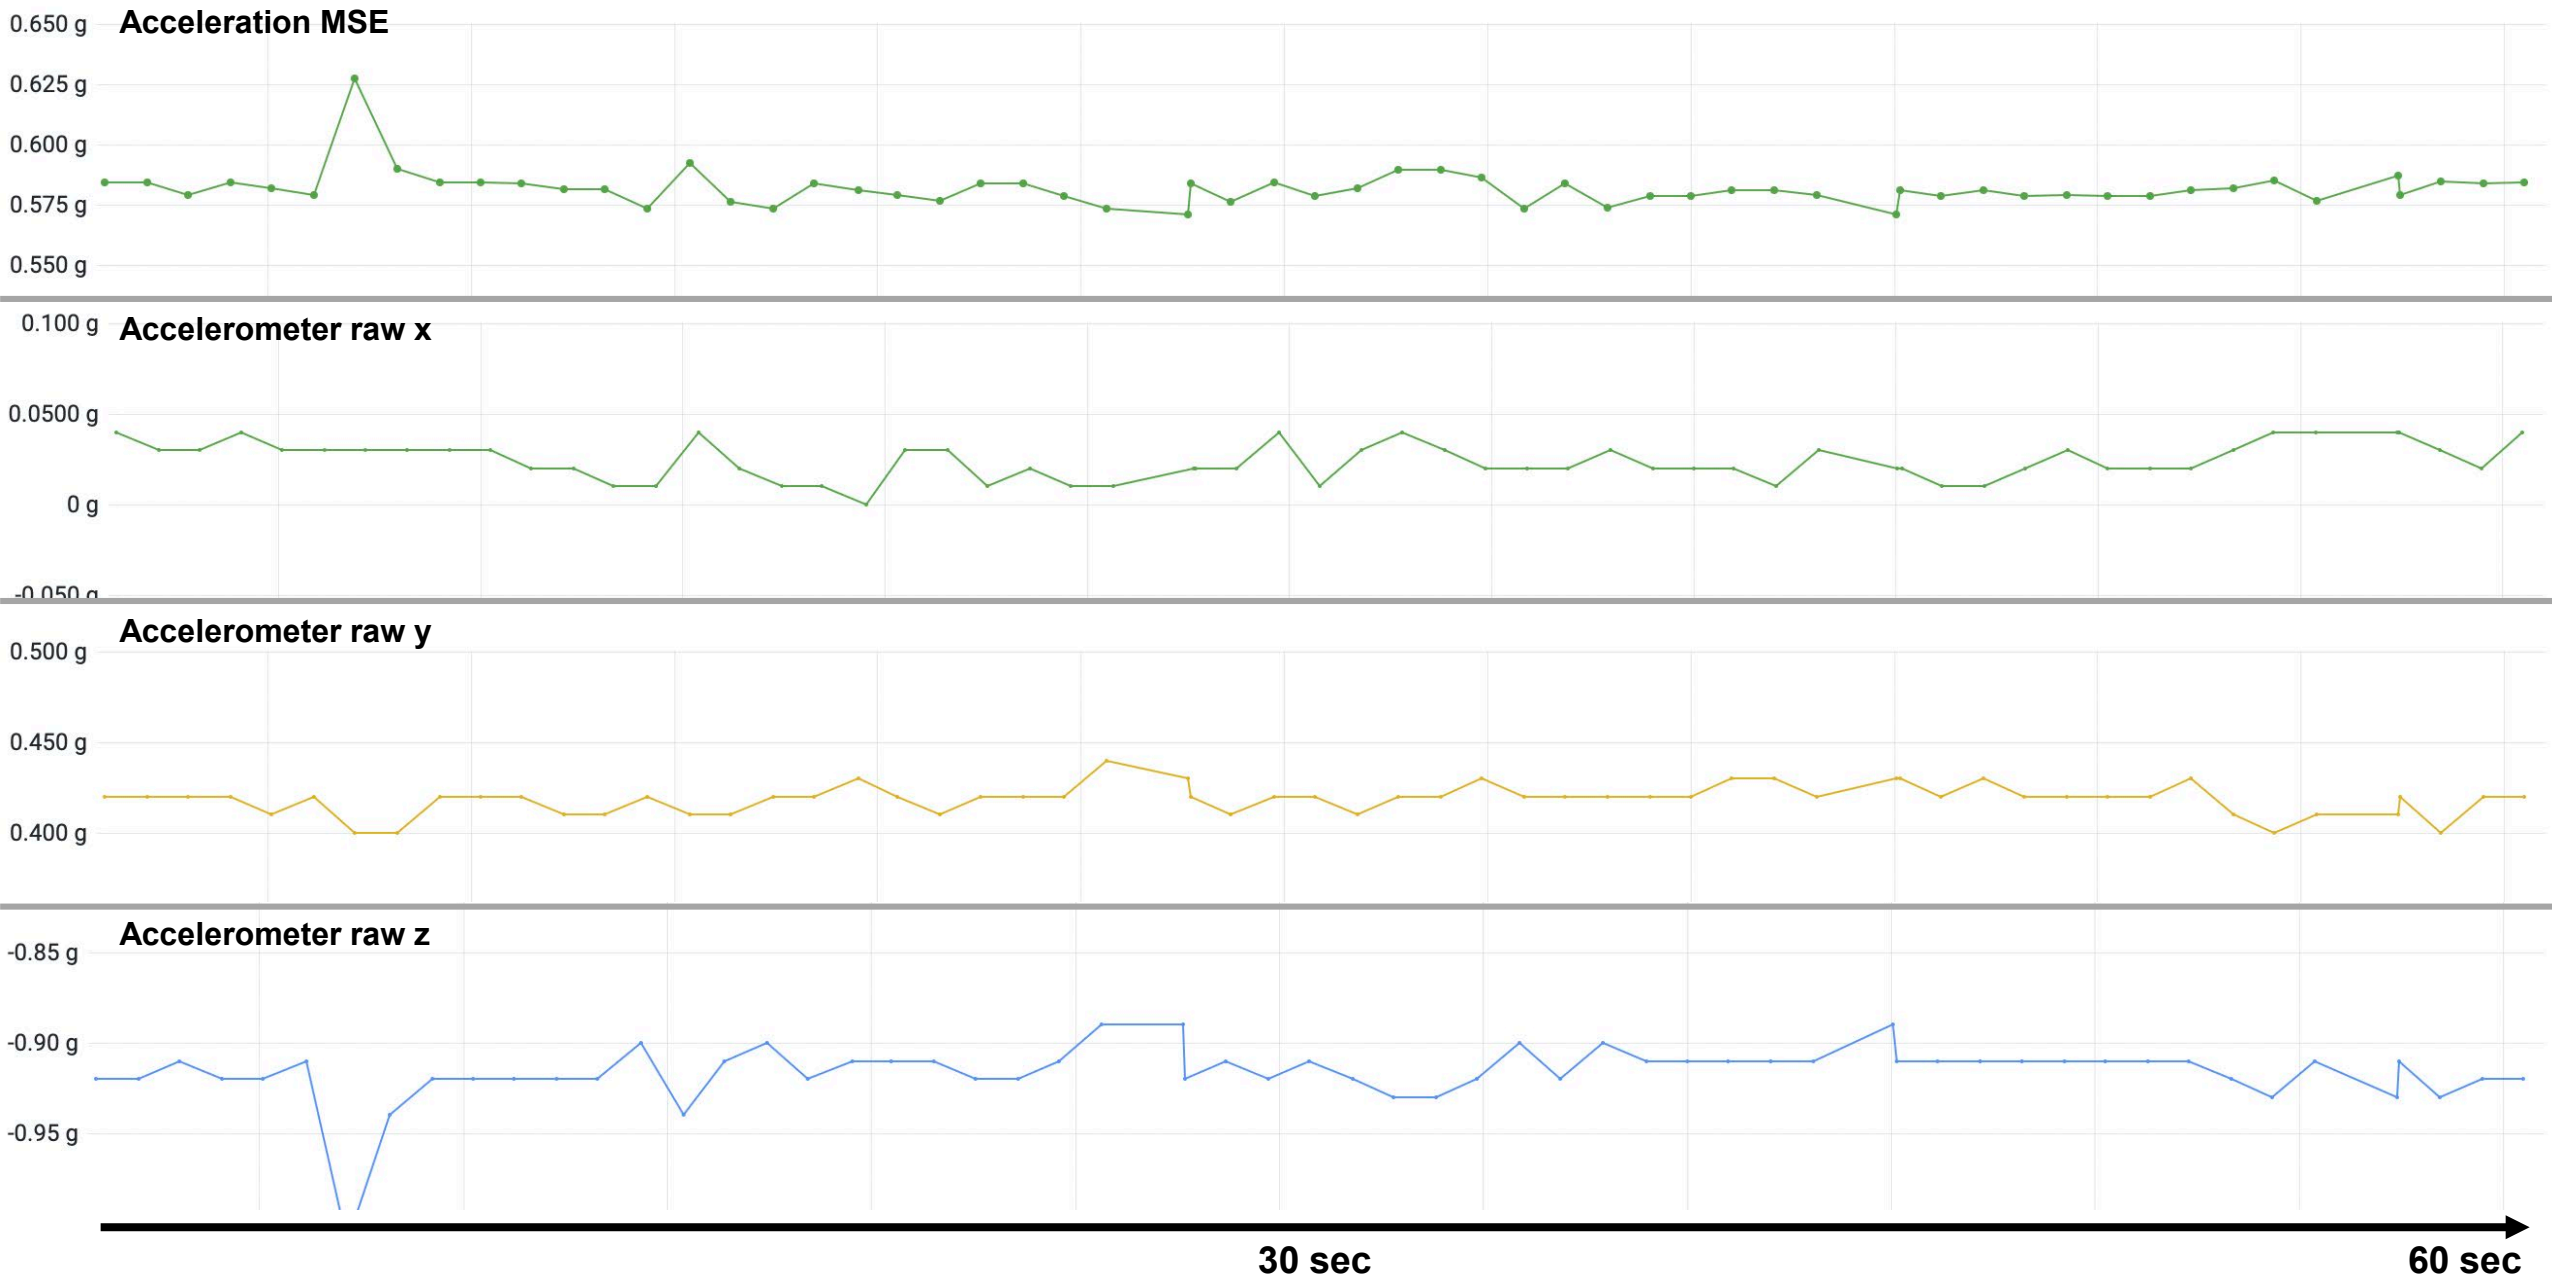


Scene 14: Subject in bed completing bed exit (here: three documented exits)

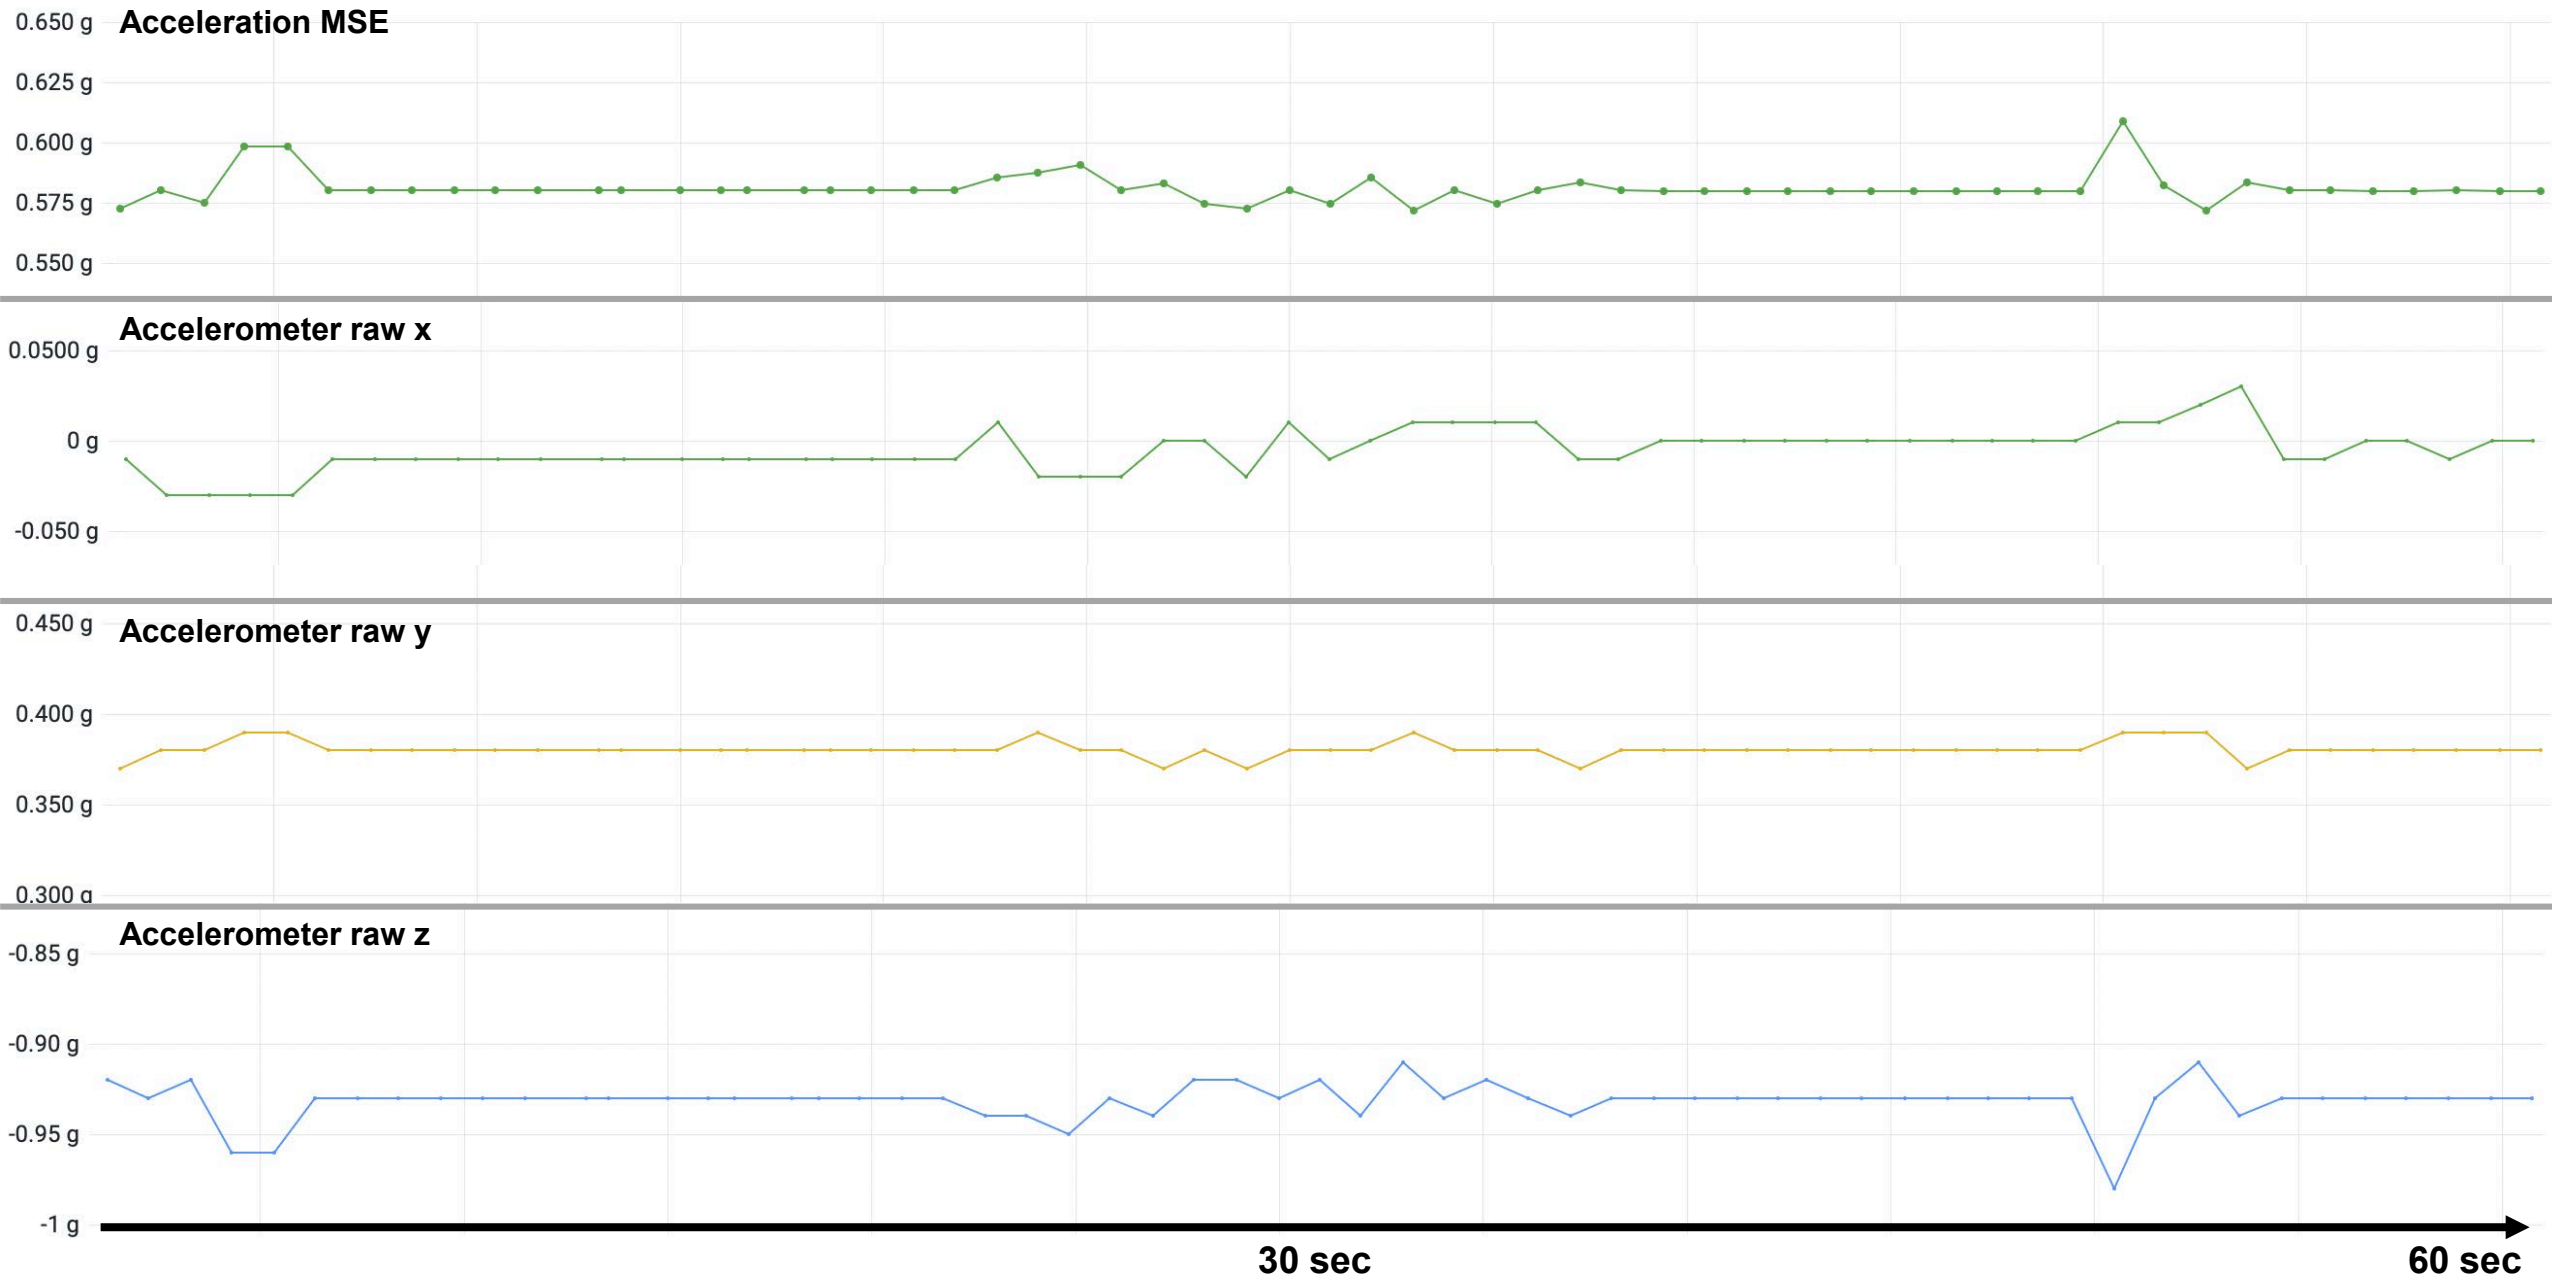


Scene 16: Subject in bed, hitting the bed with the fist

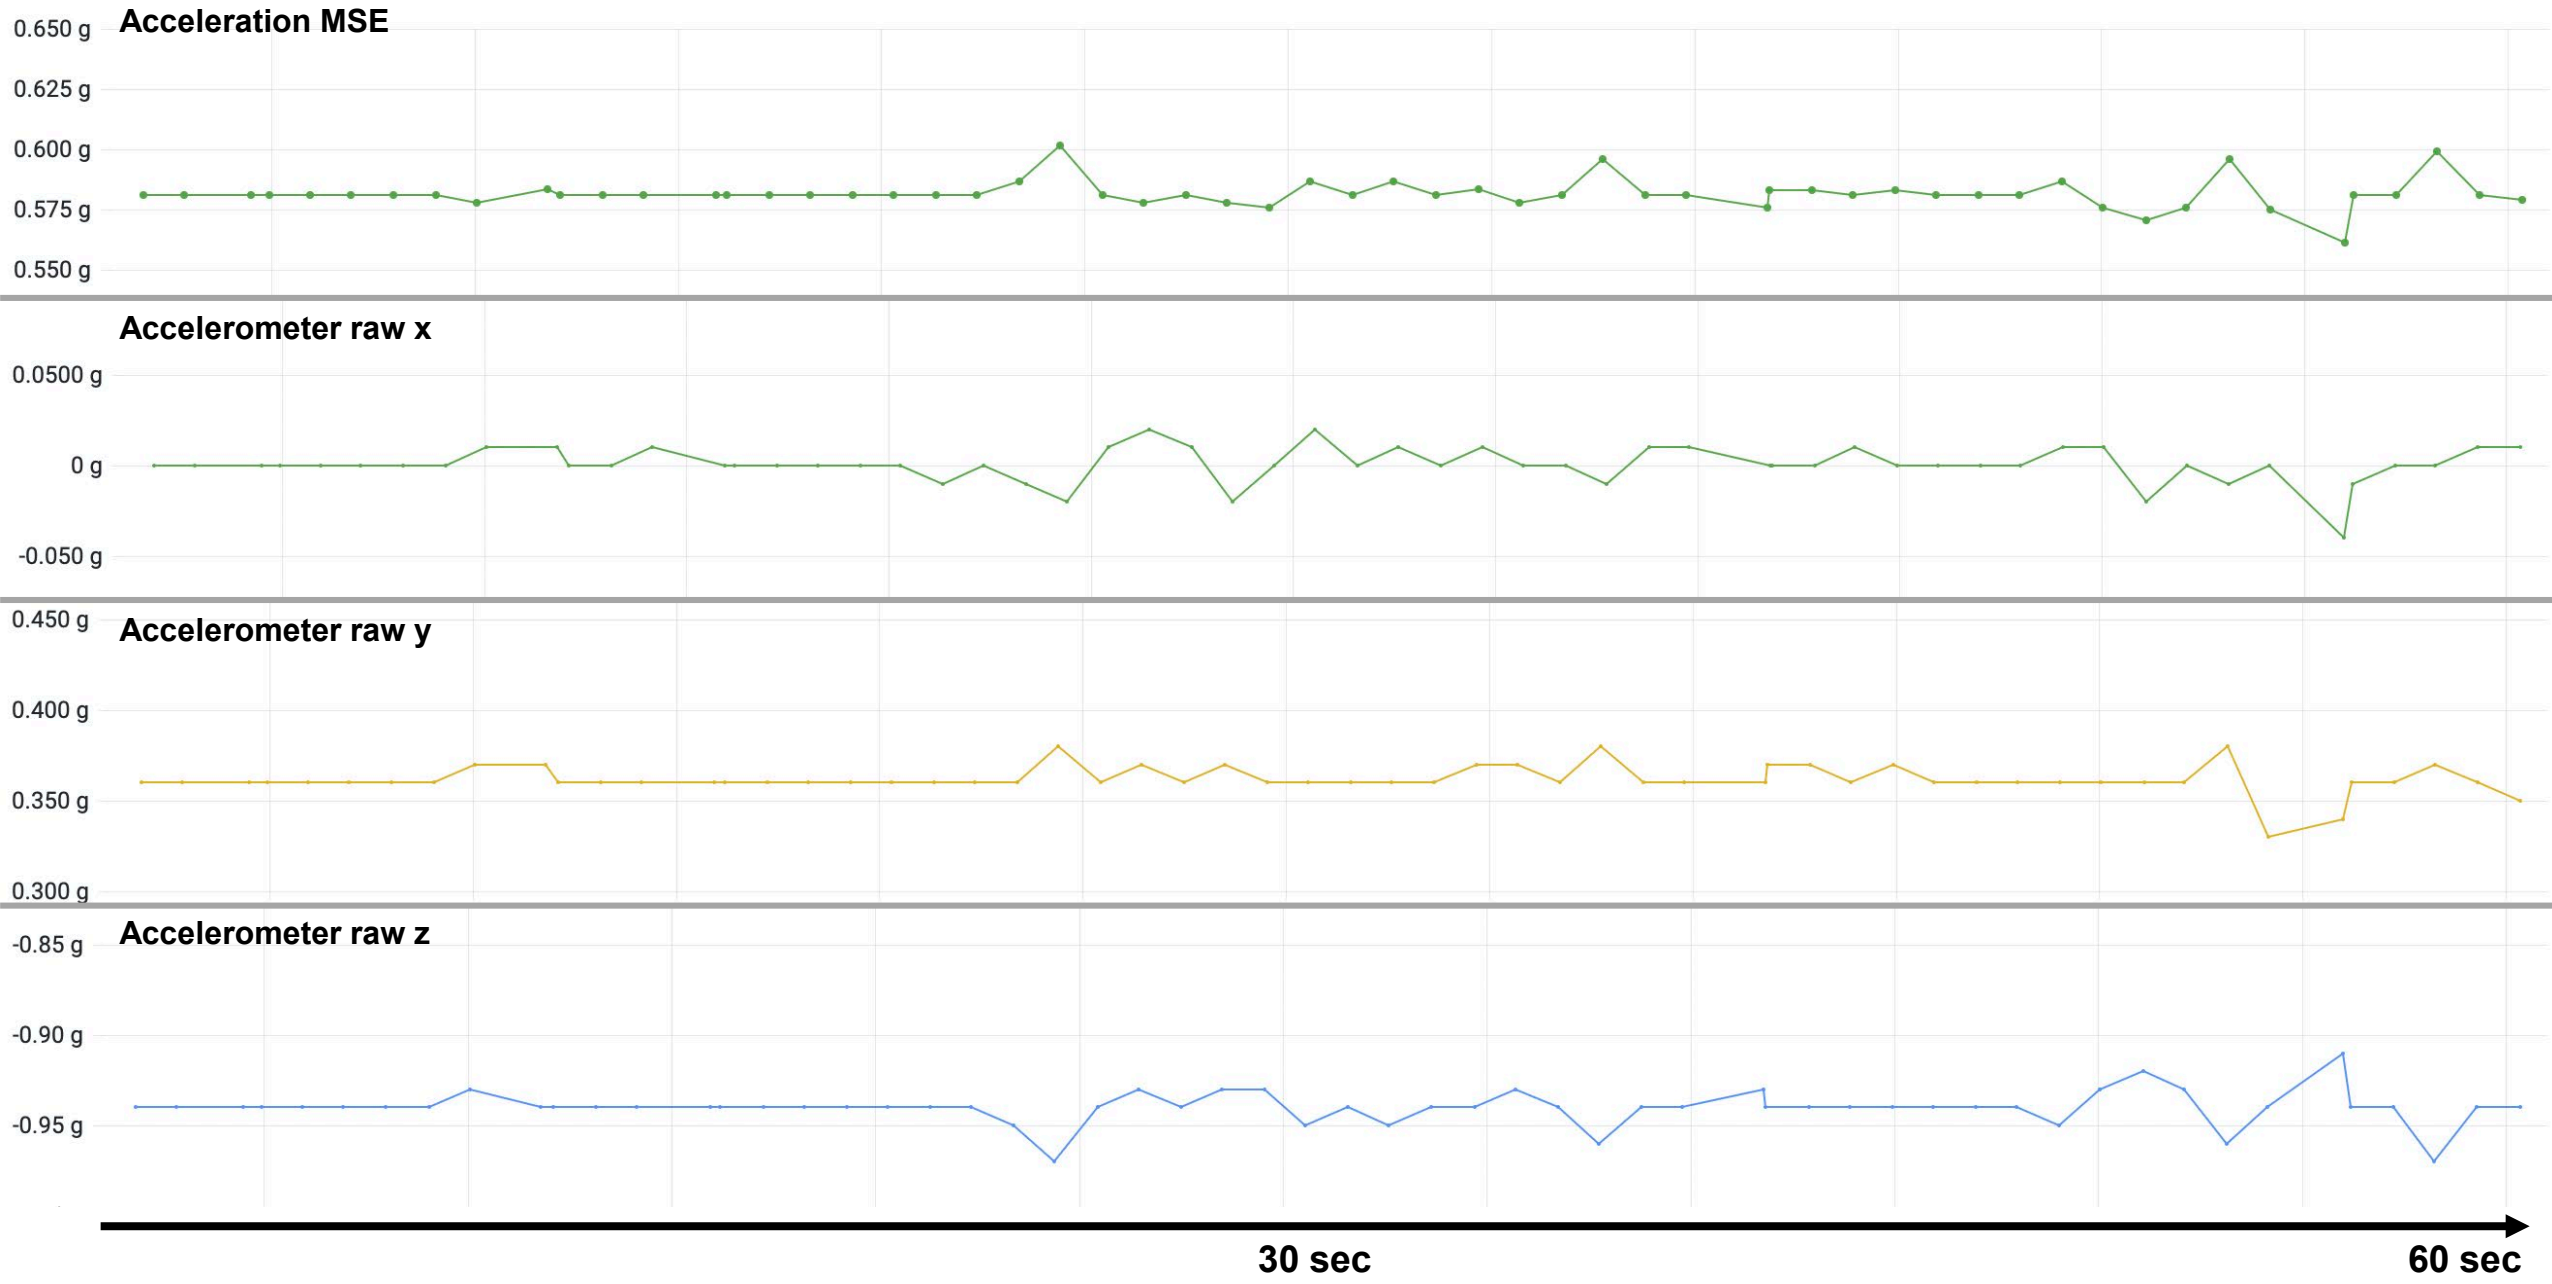


Scene 18: Subject in bed, exhibiting tremor

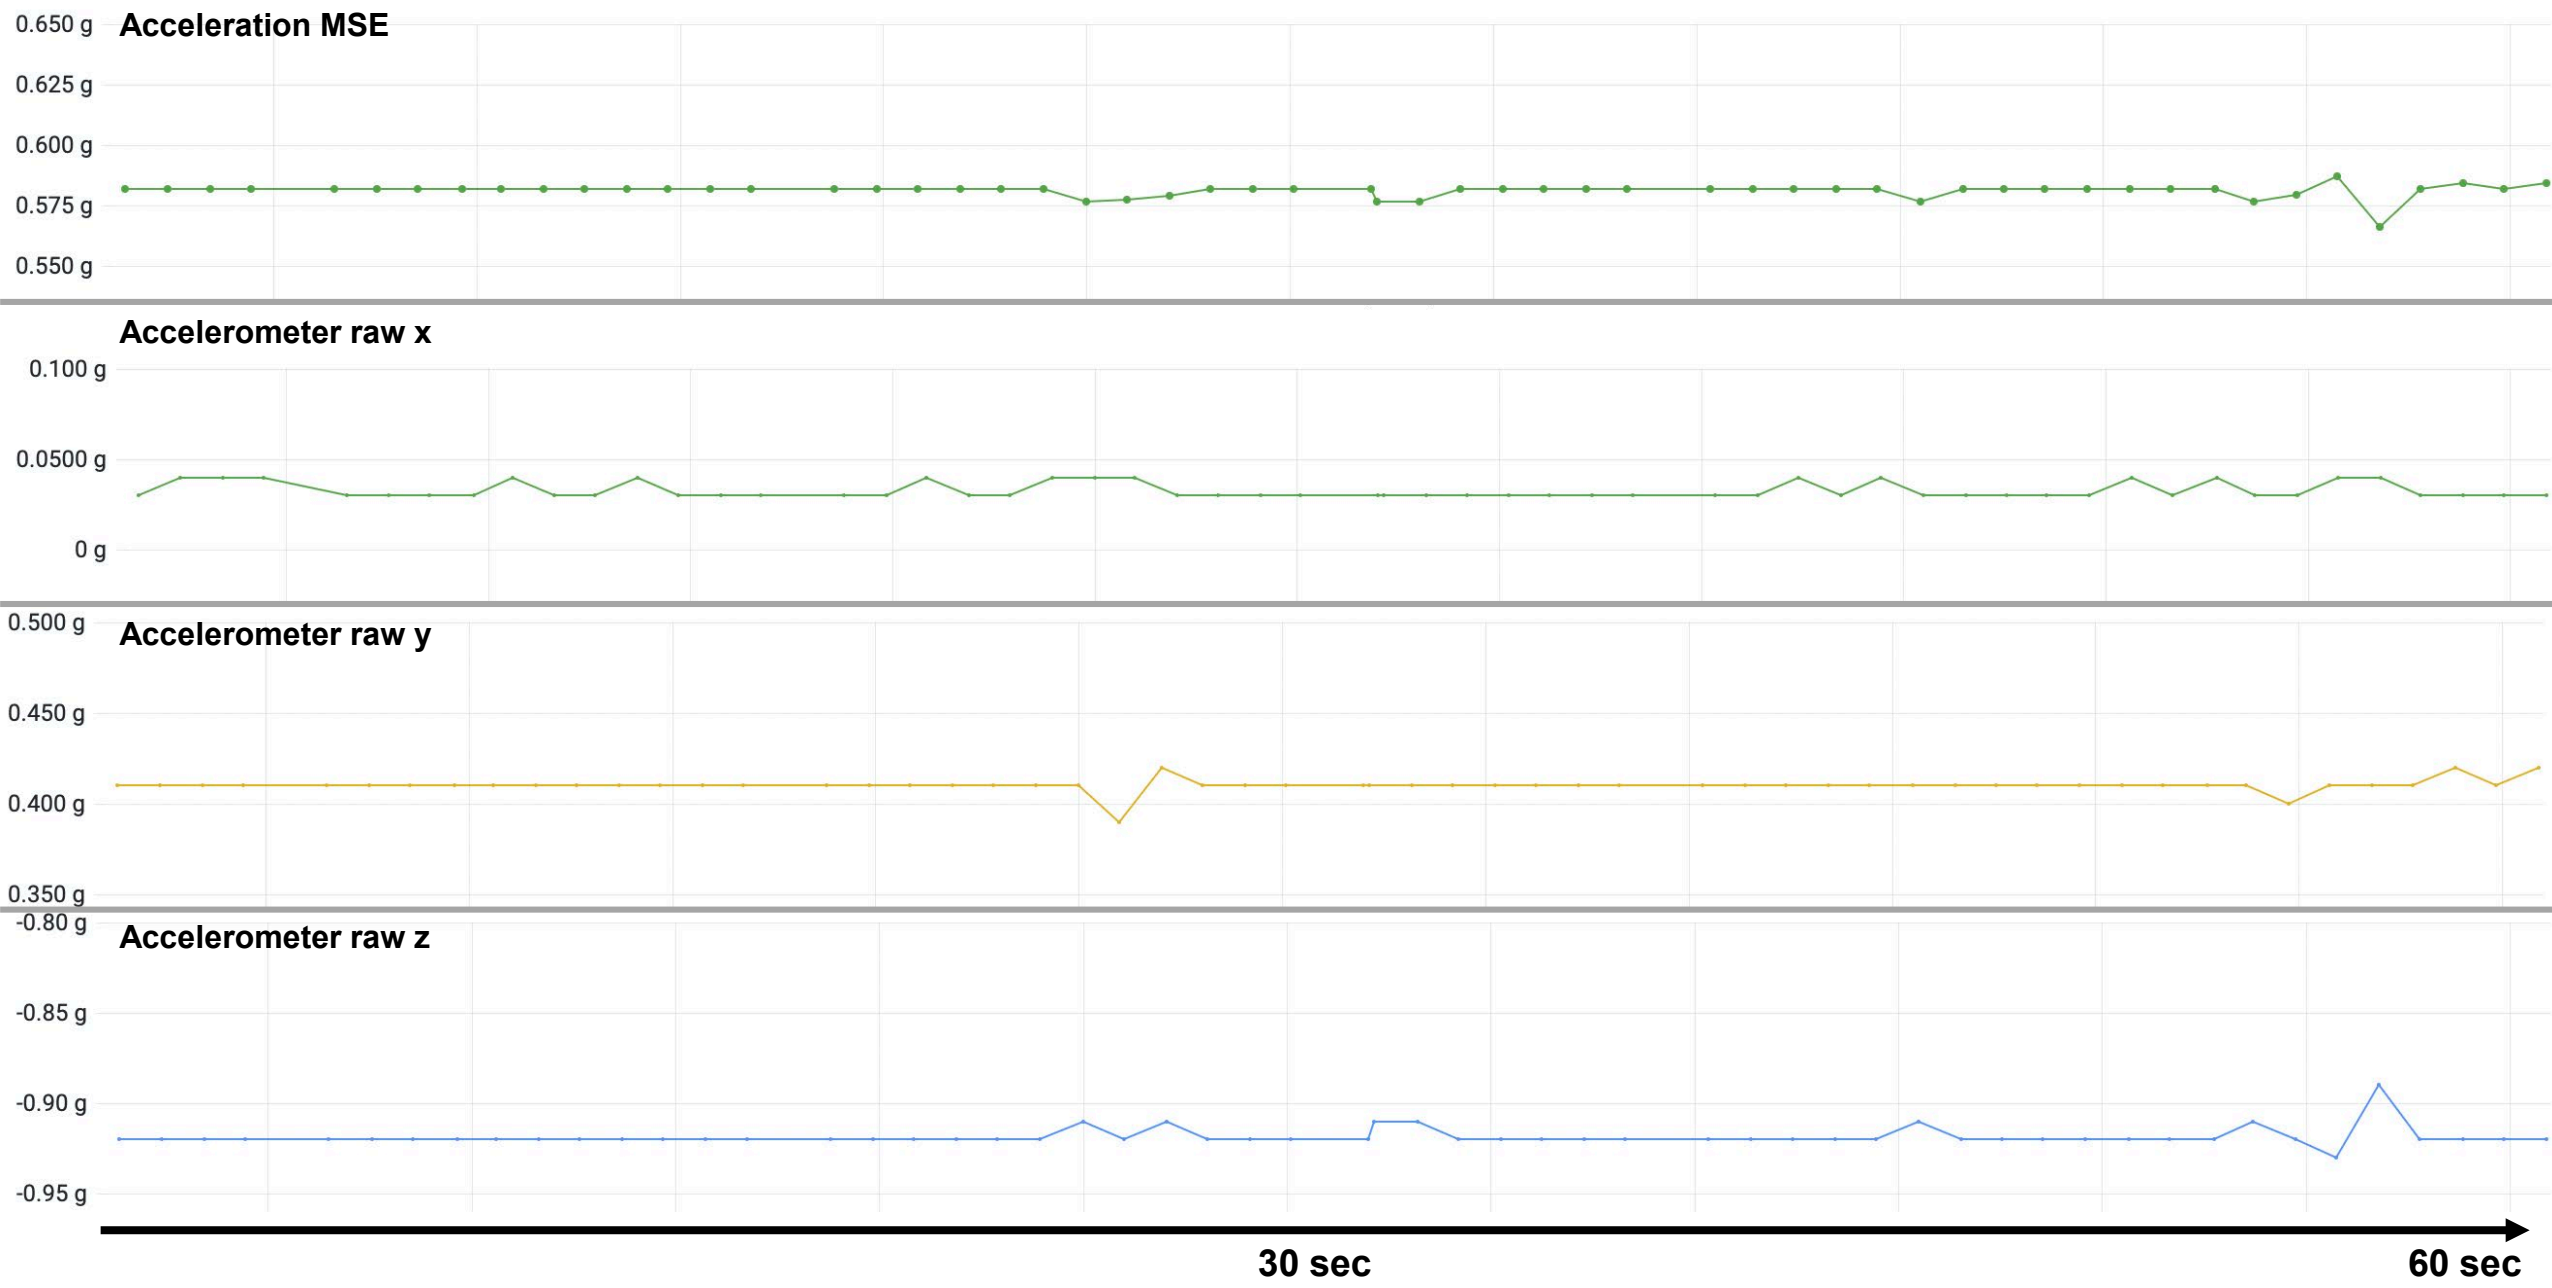


Scene 19: Joker scene – (here: cycling movements)

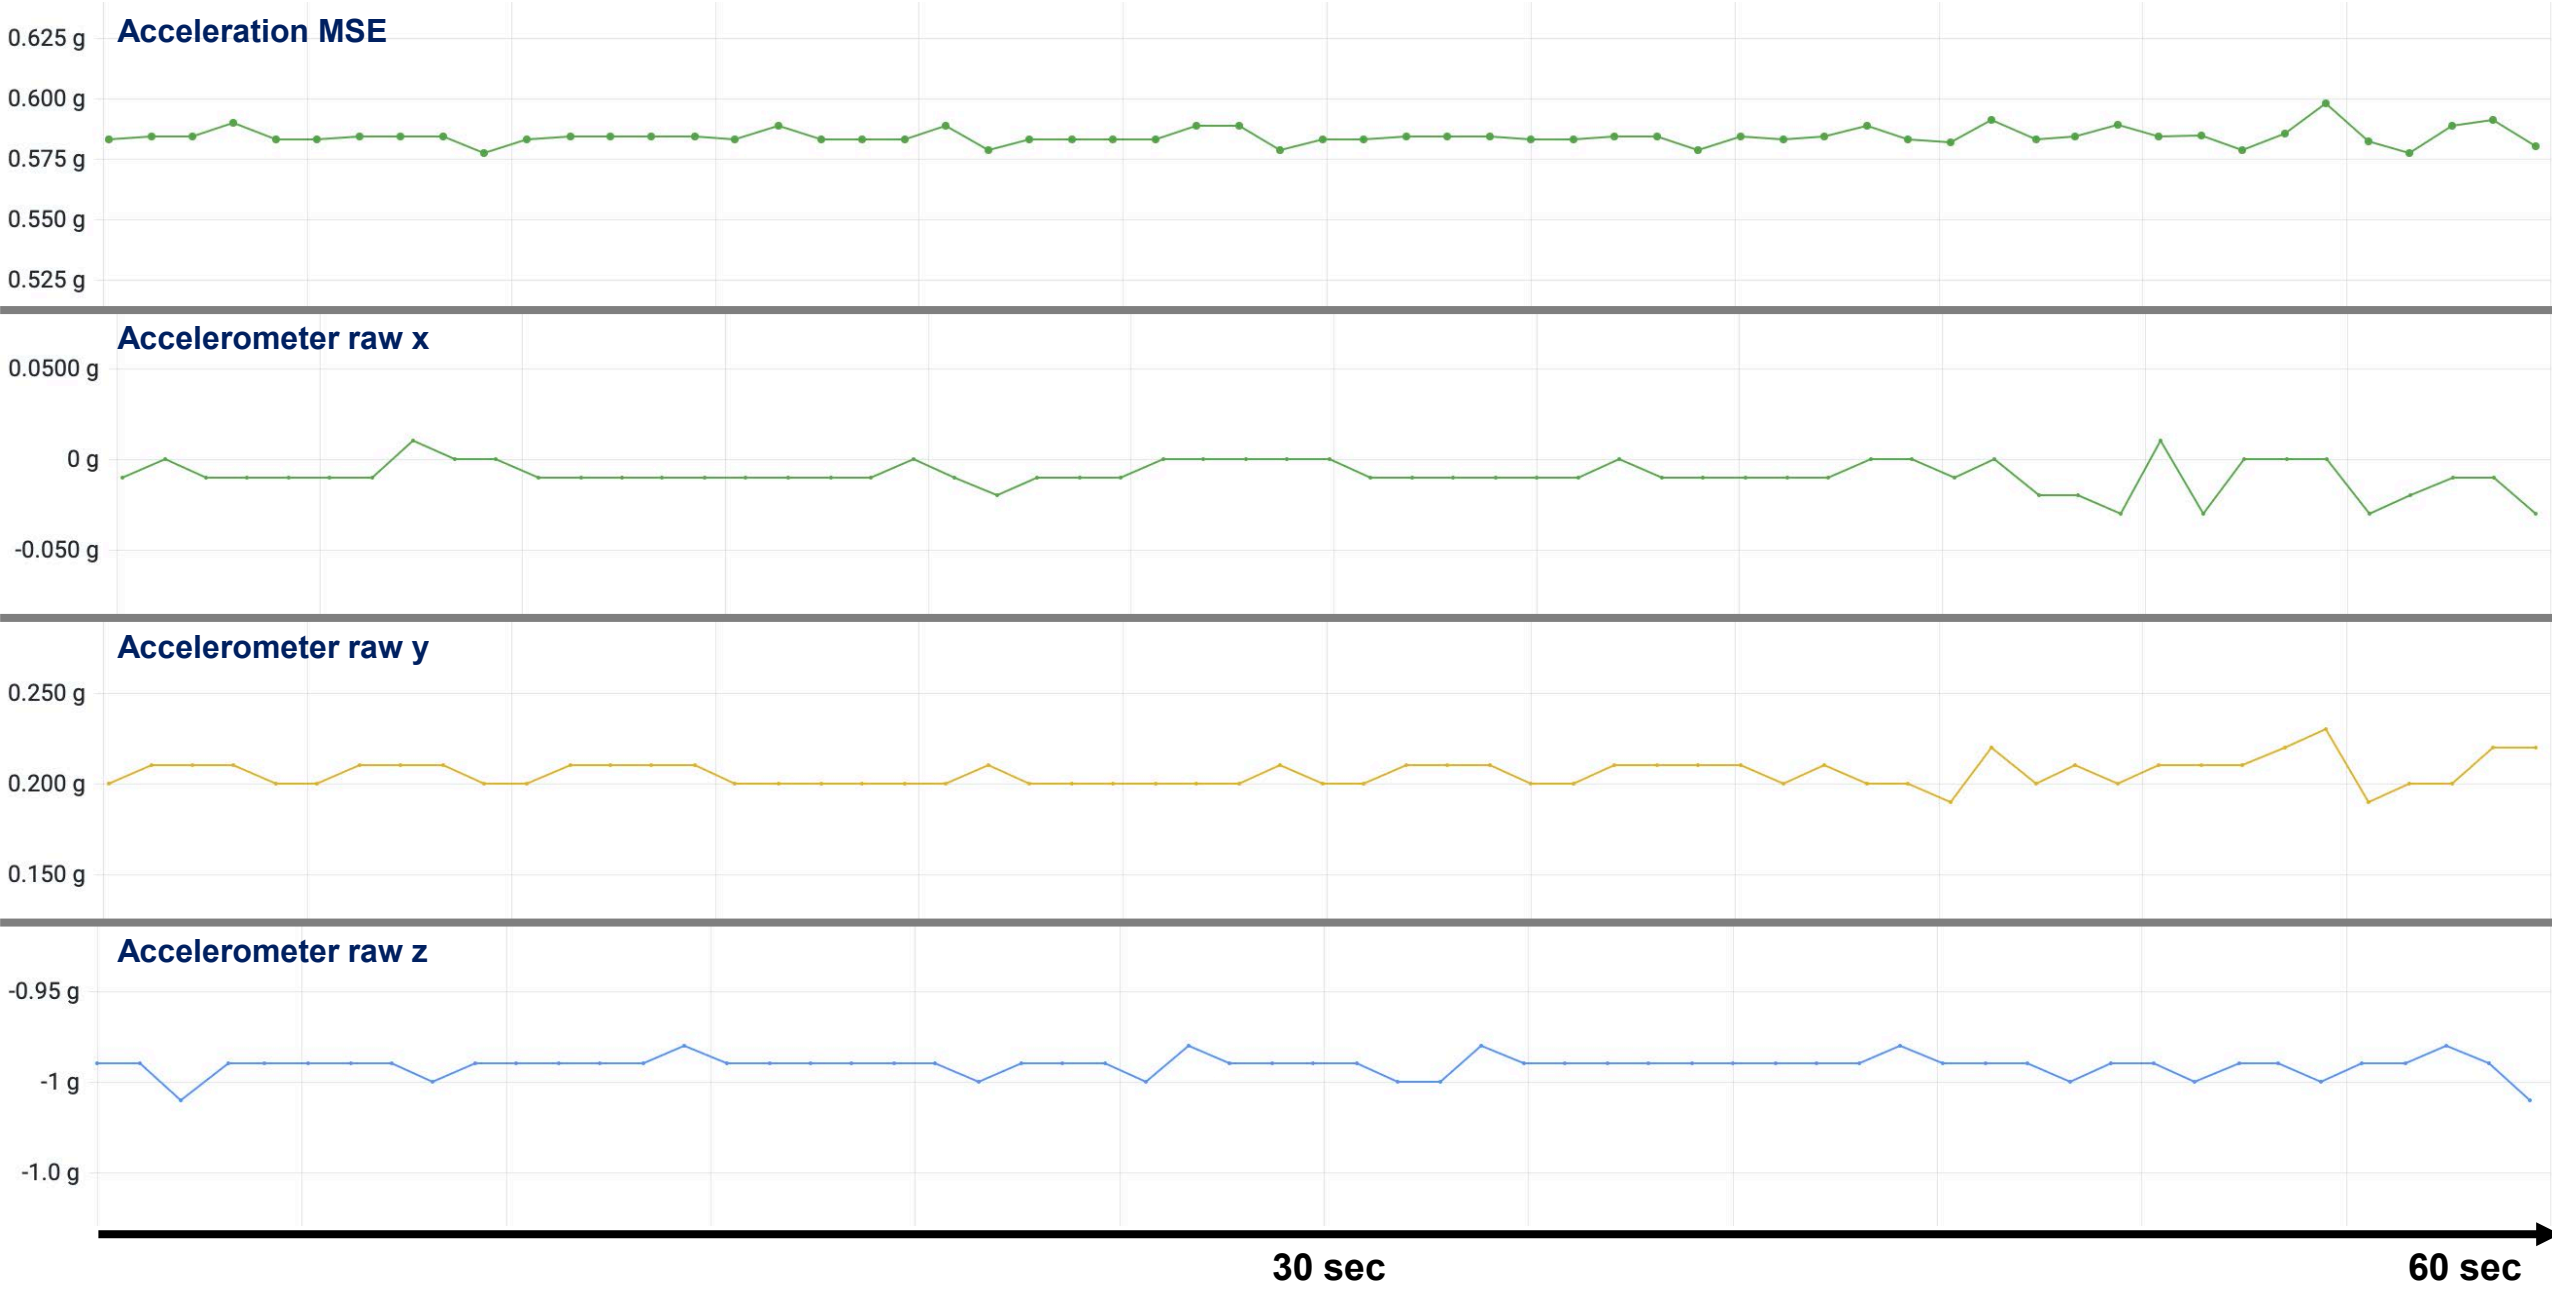


Scene 20: Subject in bed, lying relaxed

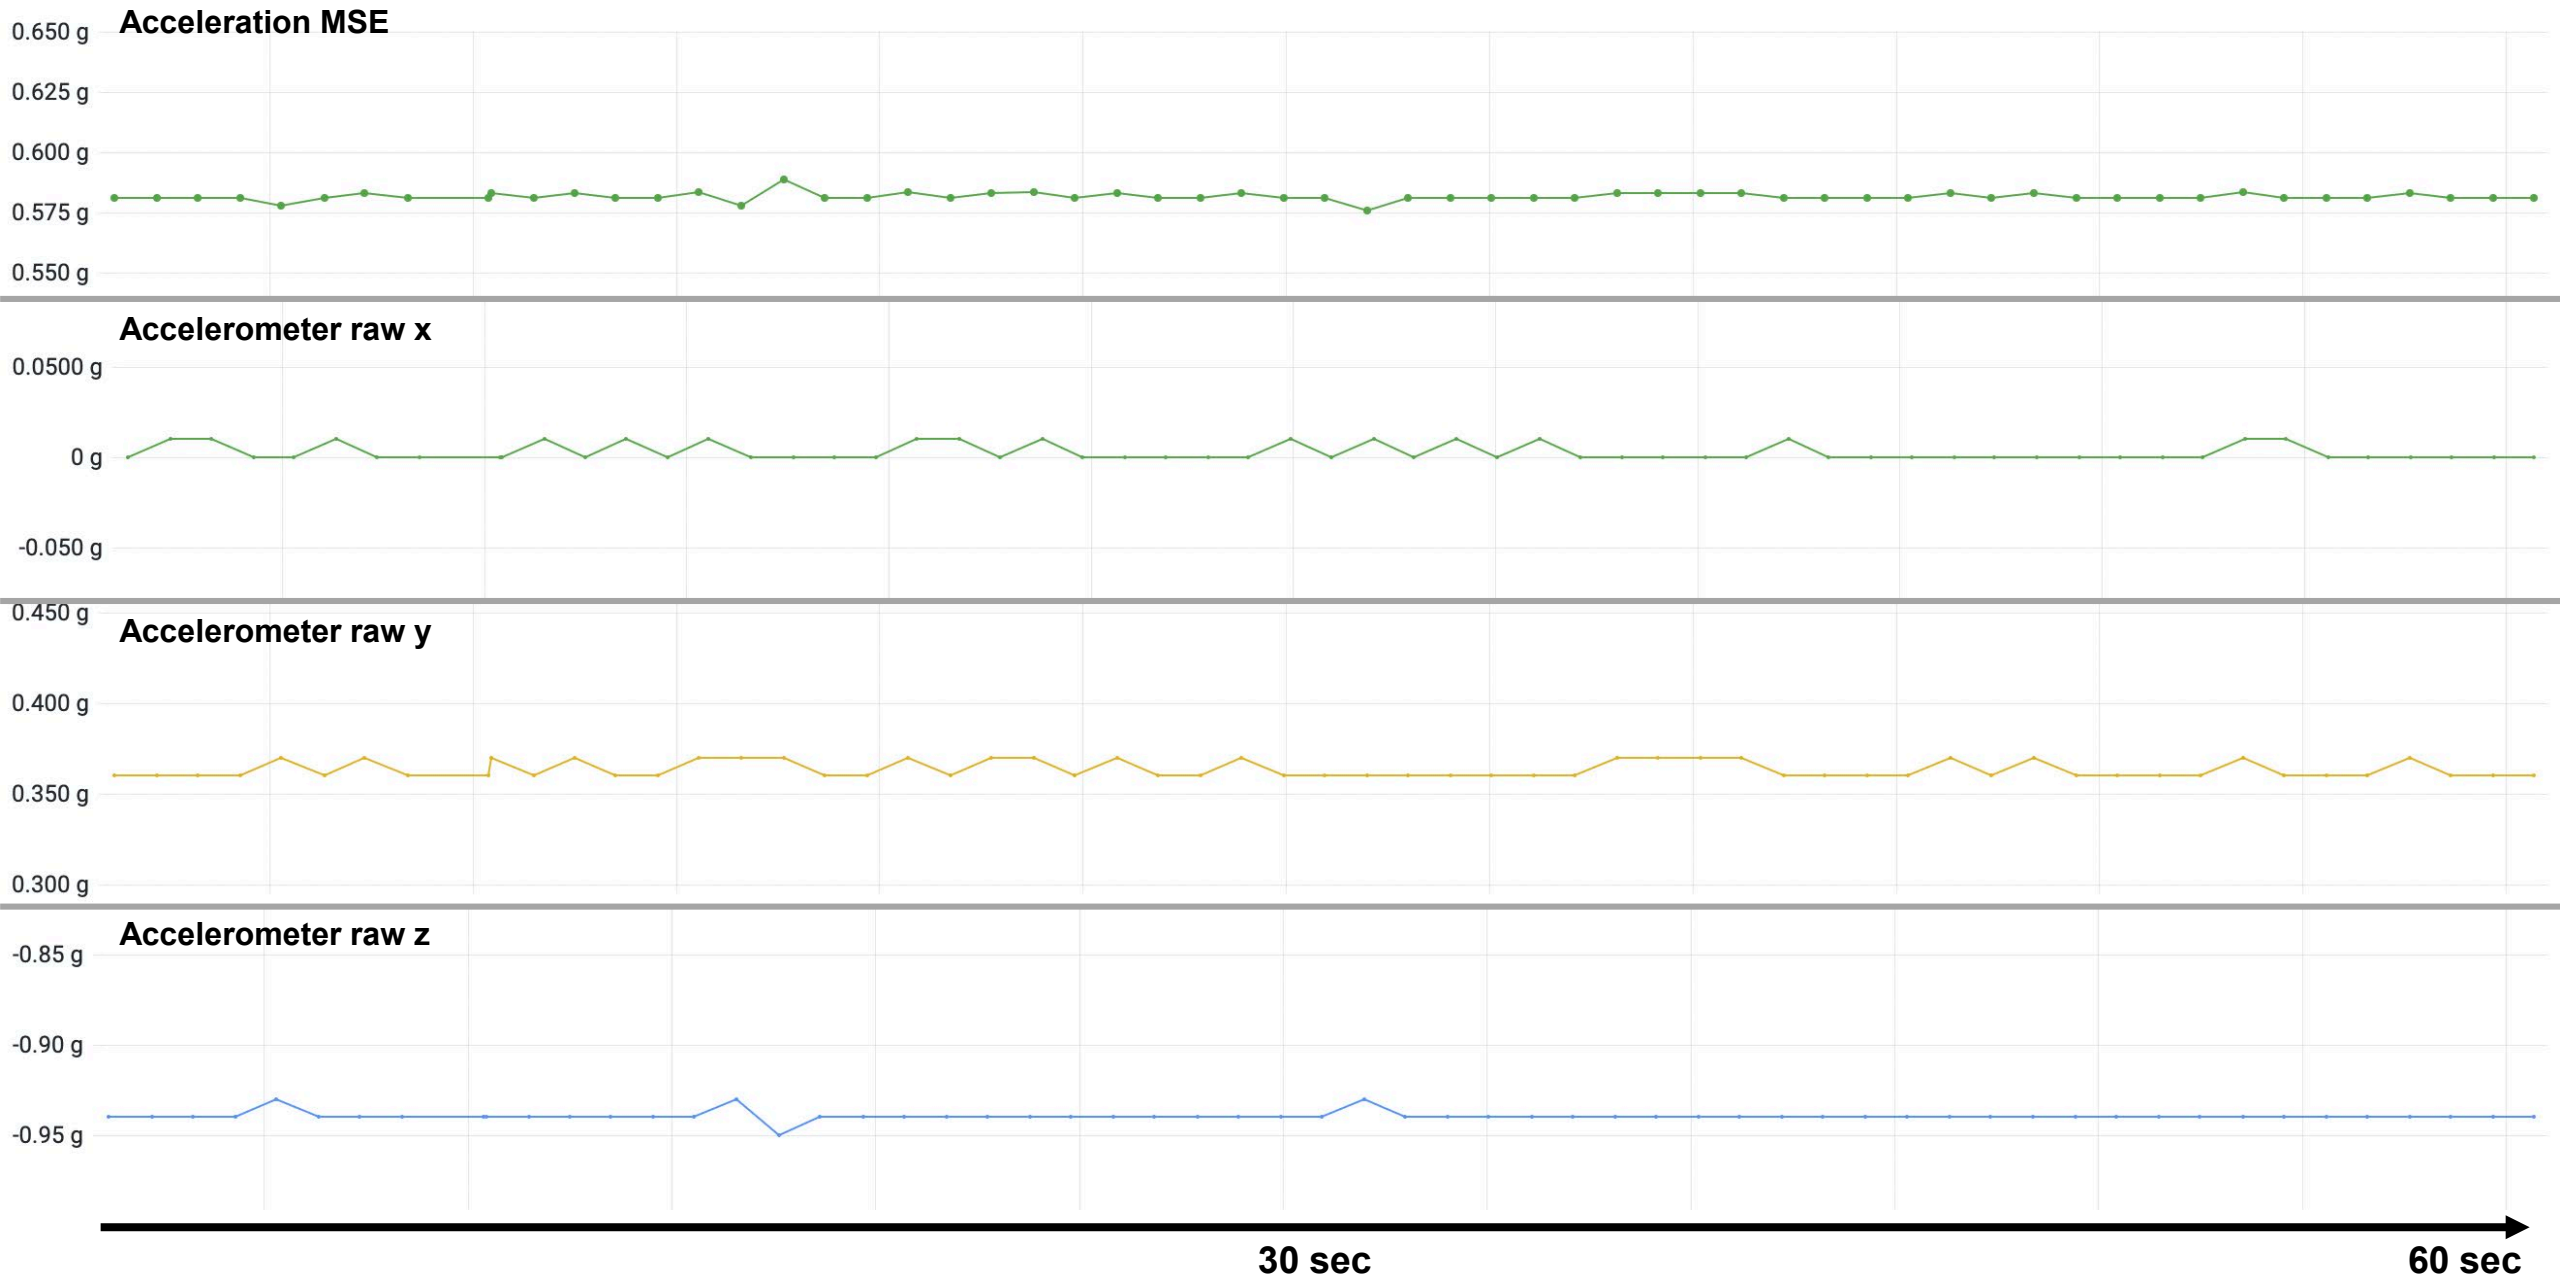

Scene 21: Subject lying in bed motionless, vibrating mobile phone

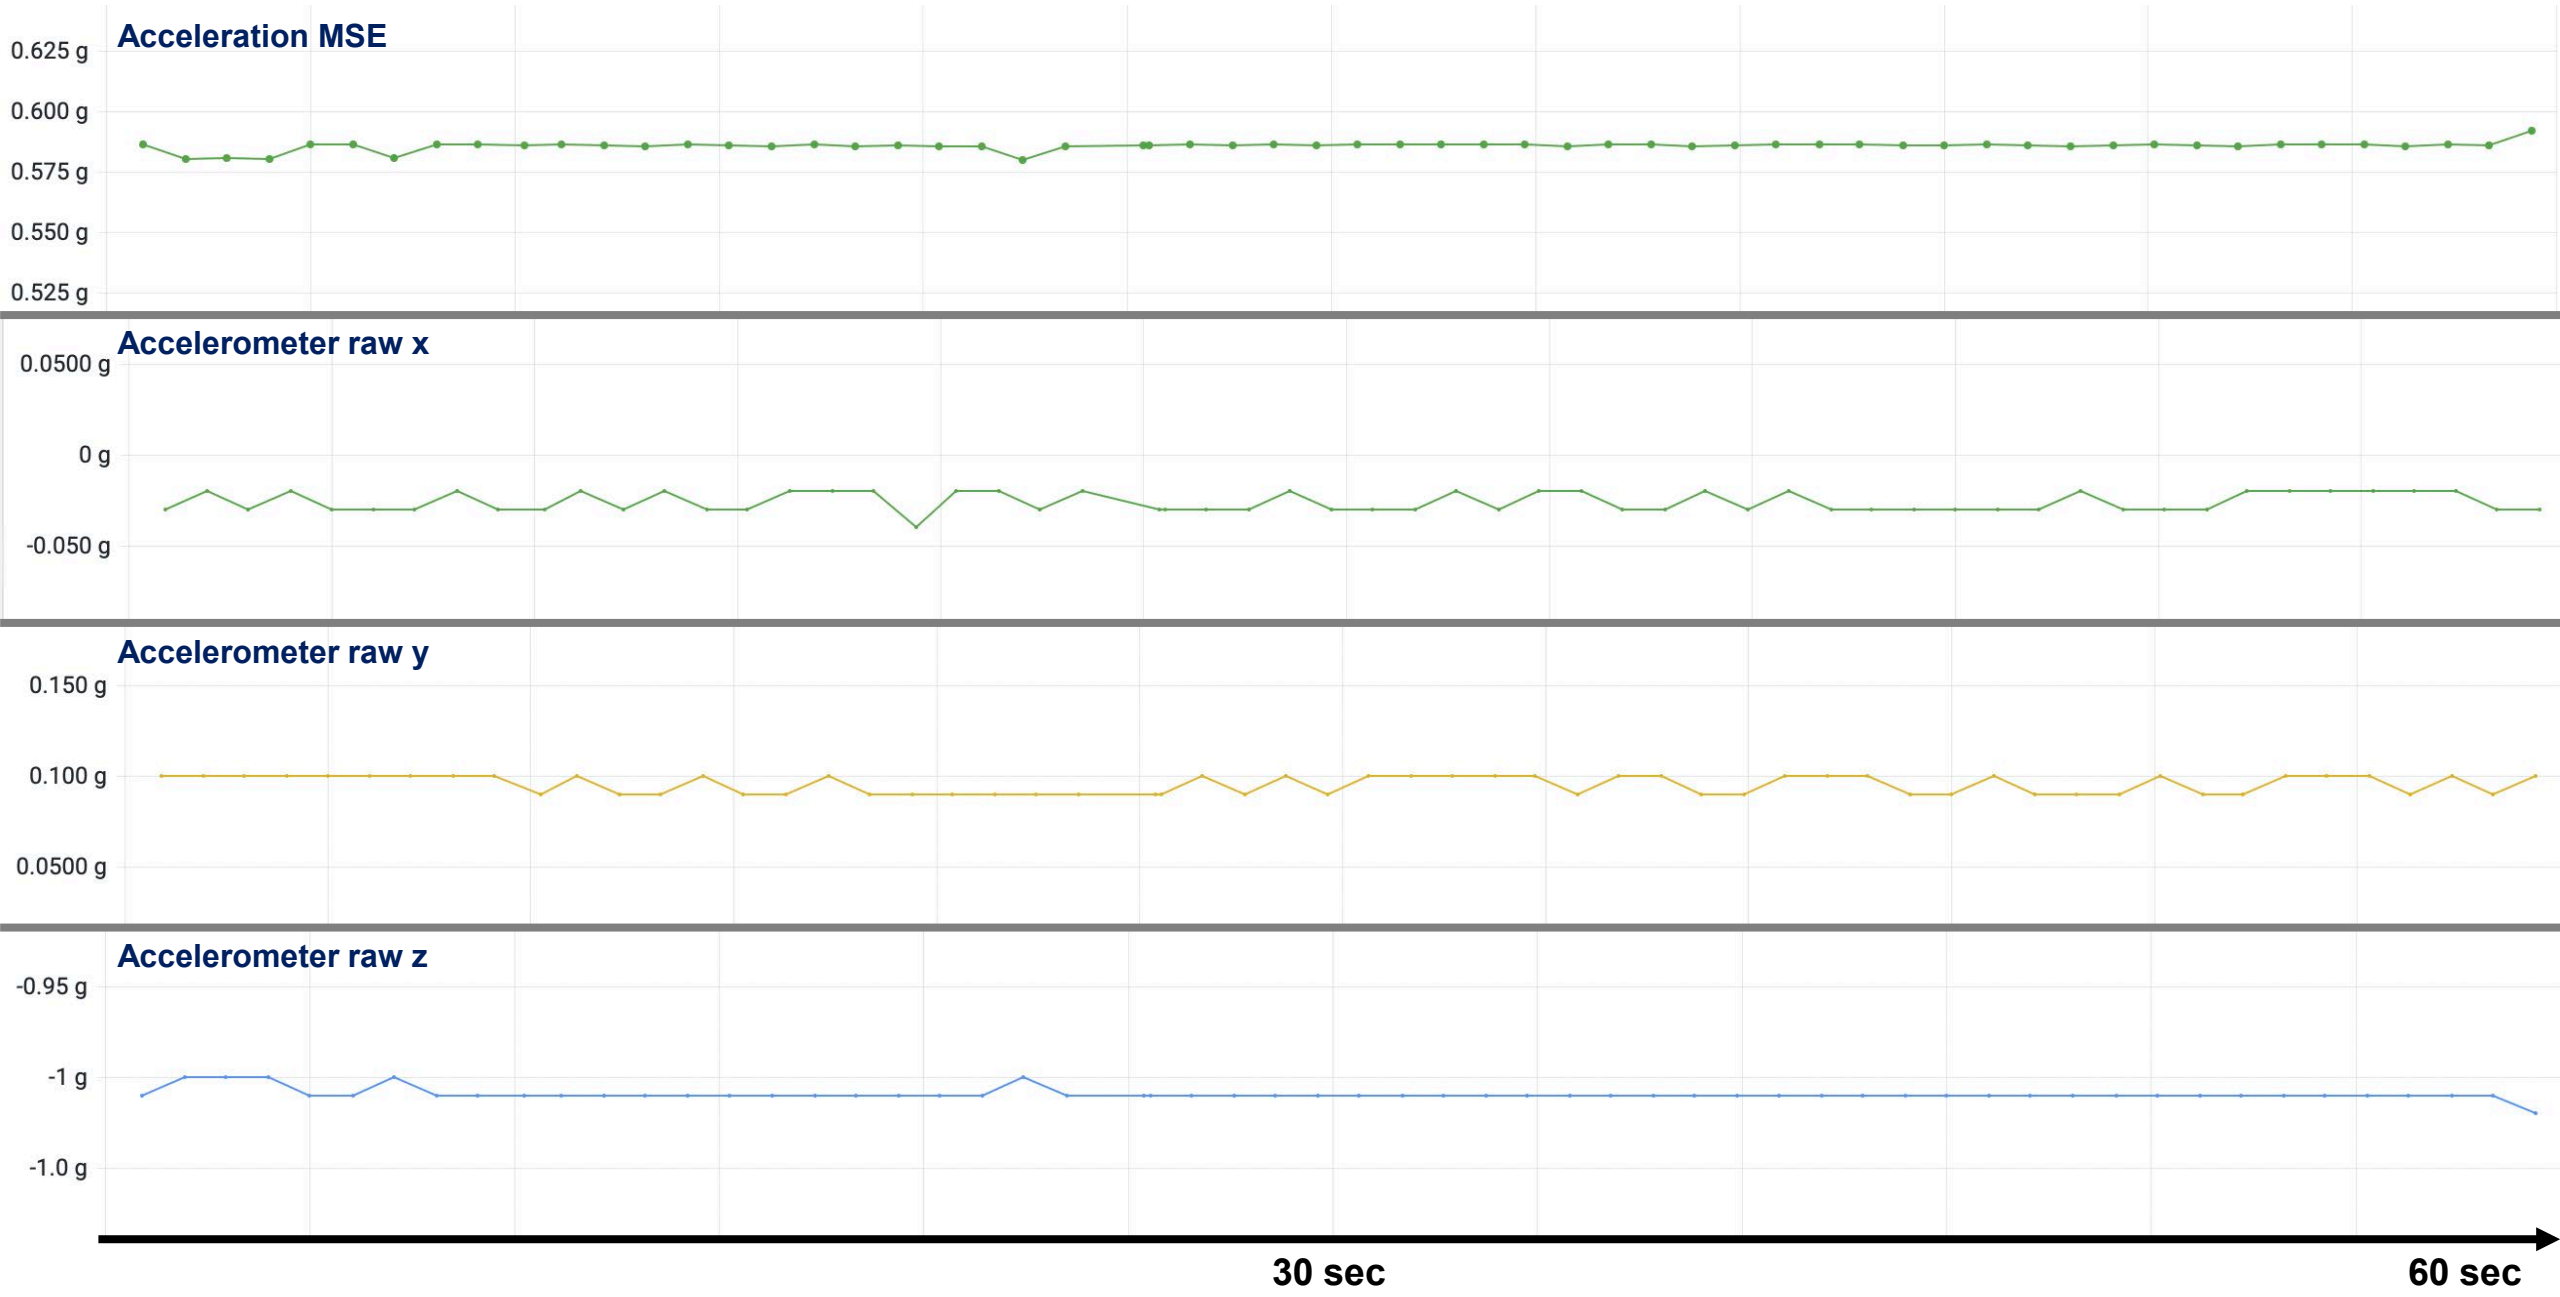


Scene 22: Bed empty, vibrating mobile phone

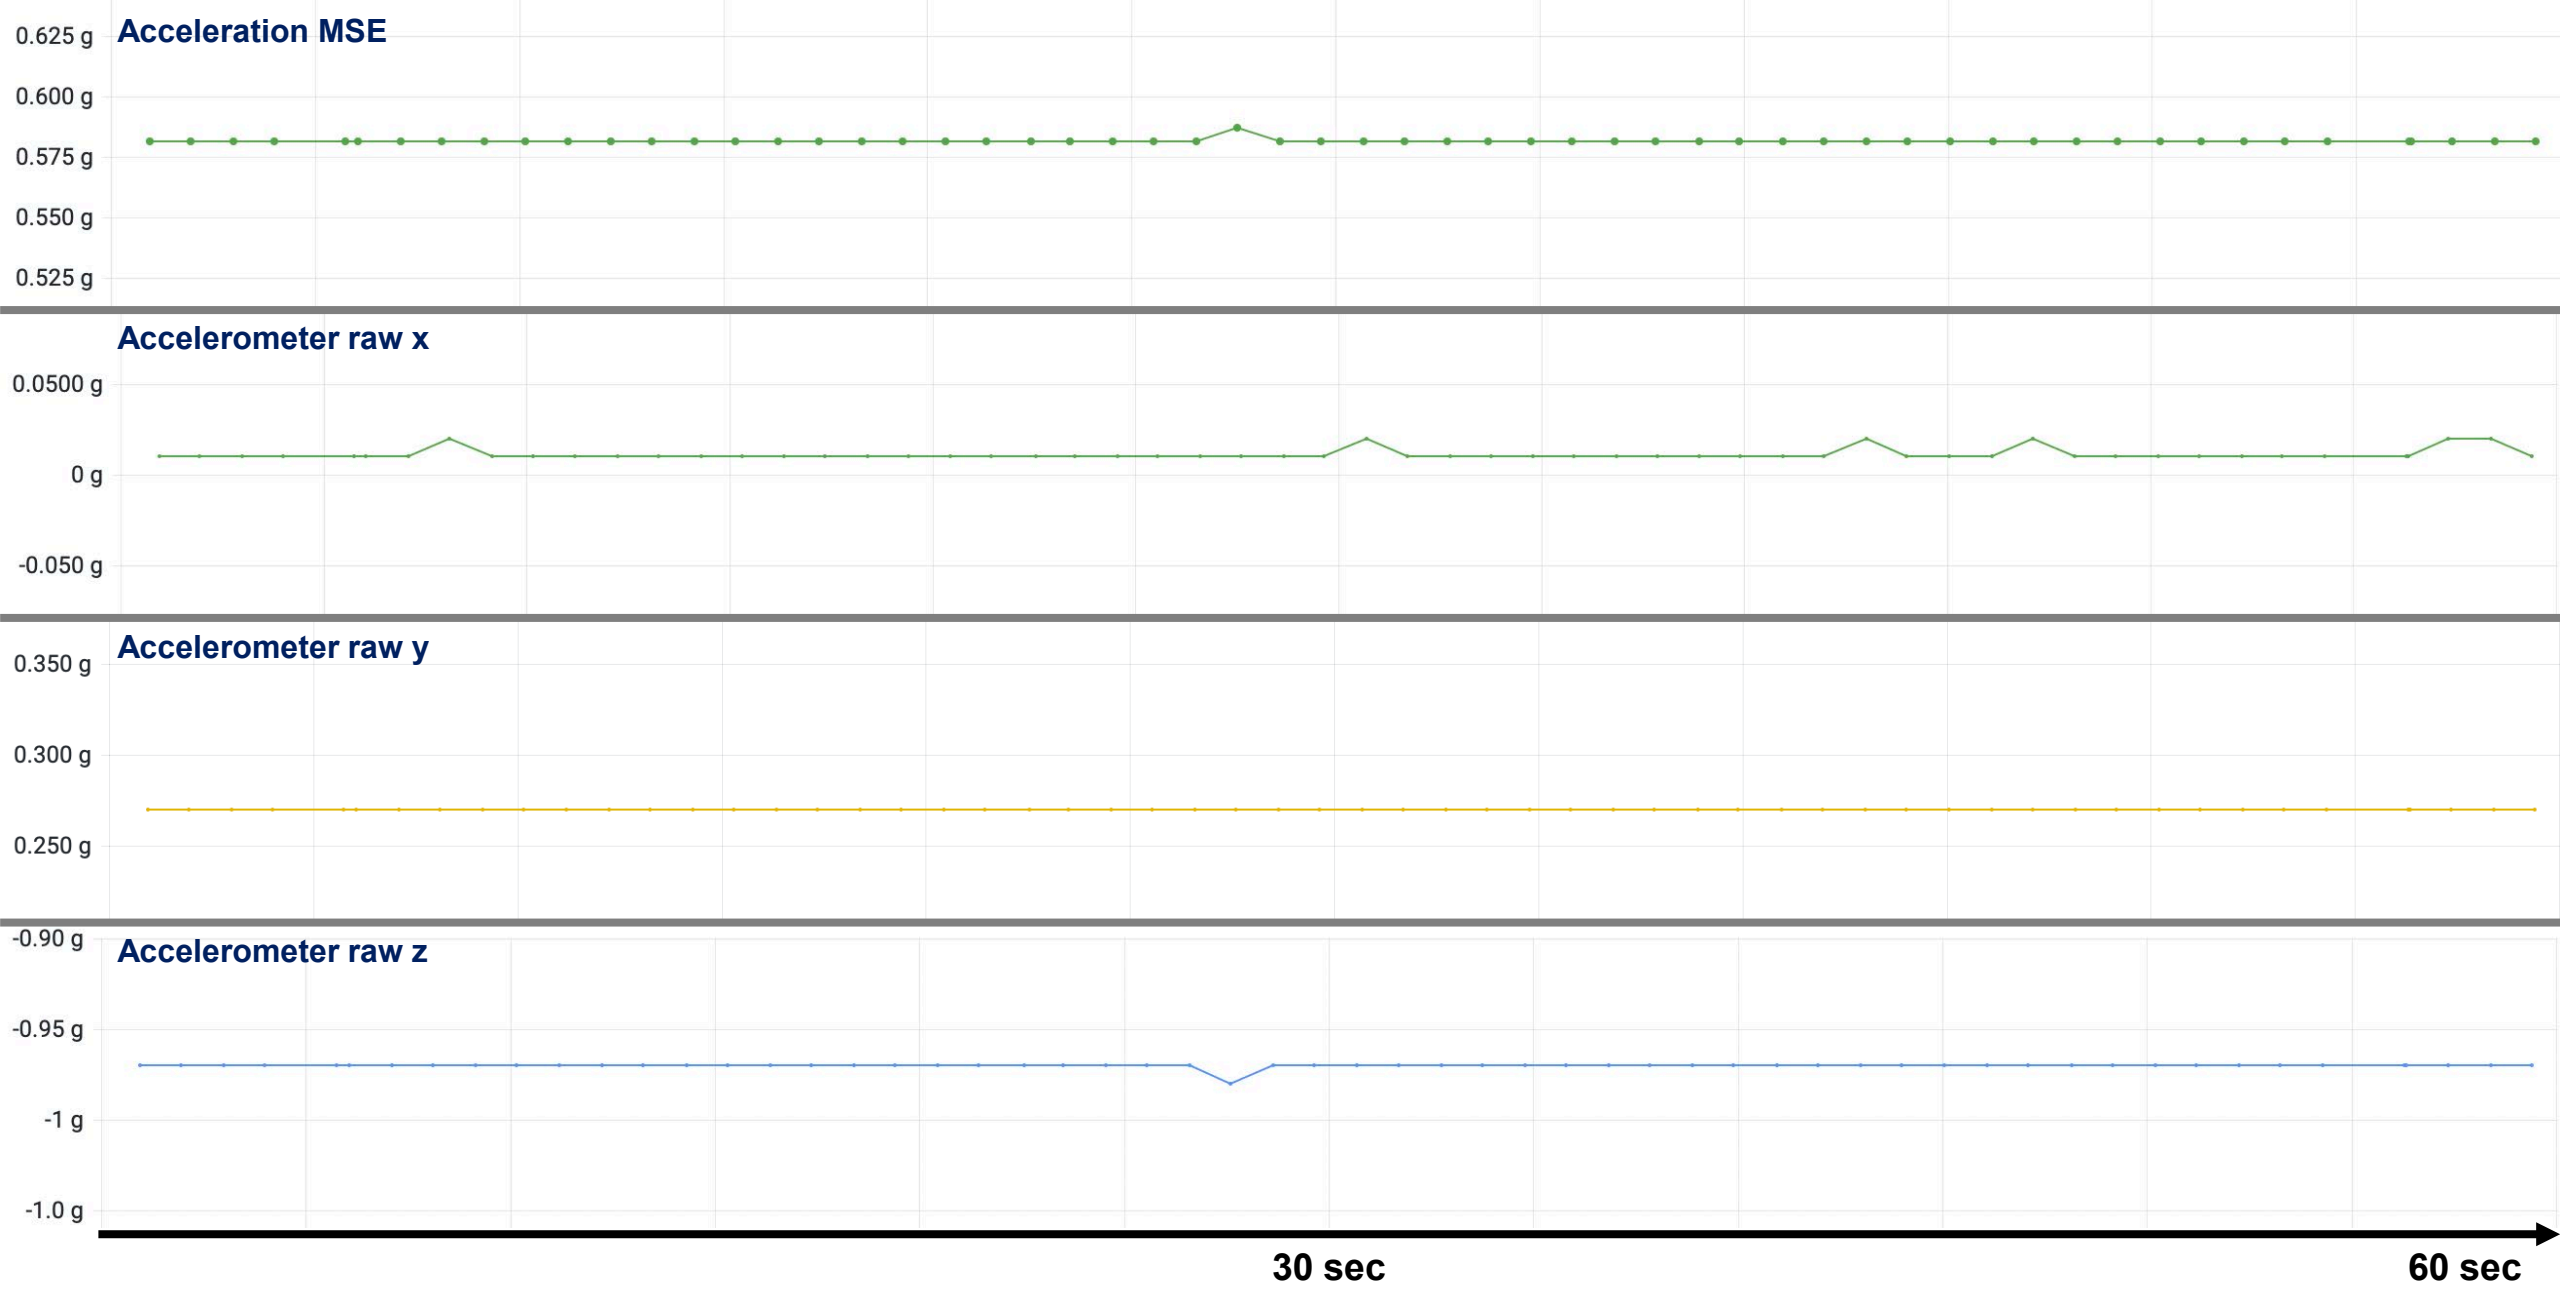


Three exemplary Scenes resulting in false positive or false negative test results by the panel


Scene 1: Bed empty. Panel classification: Scene 20. Subject in bed, lying relaxed

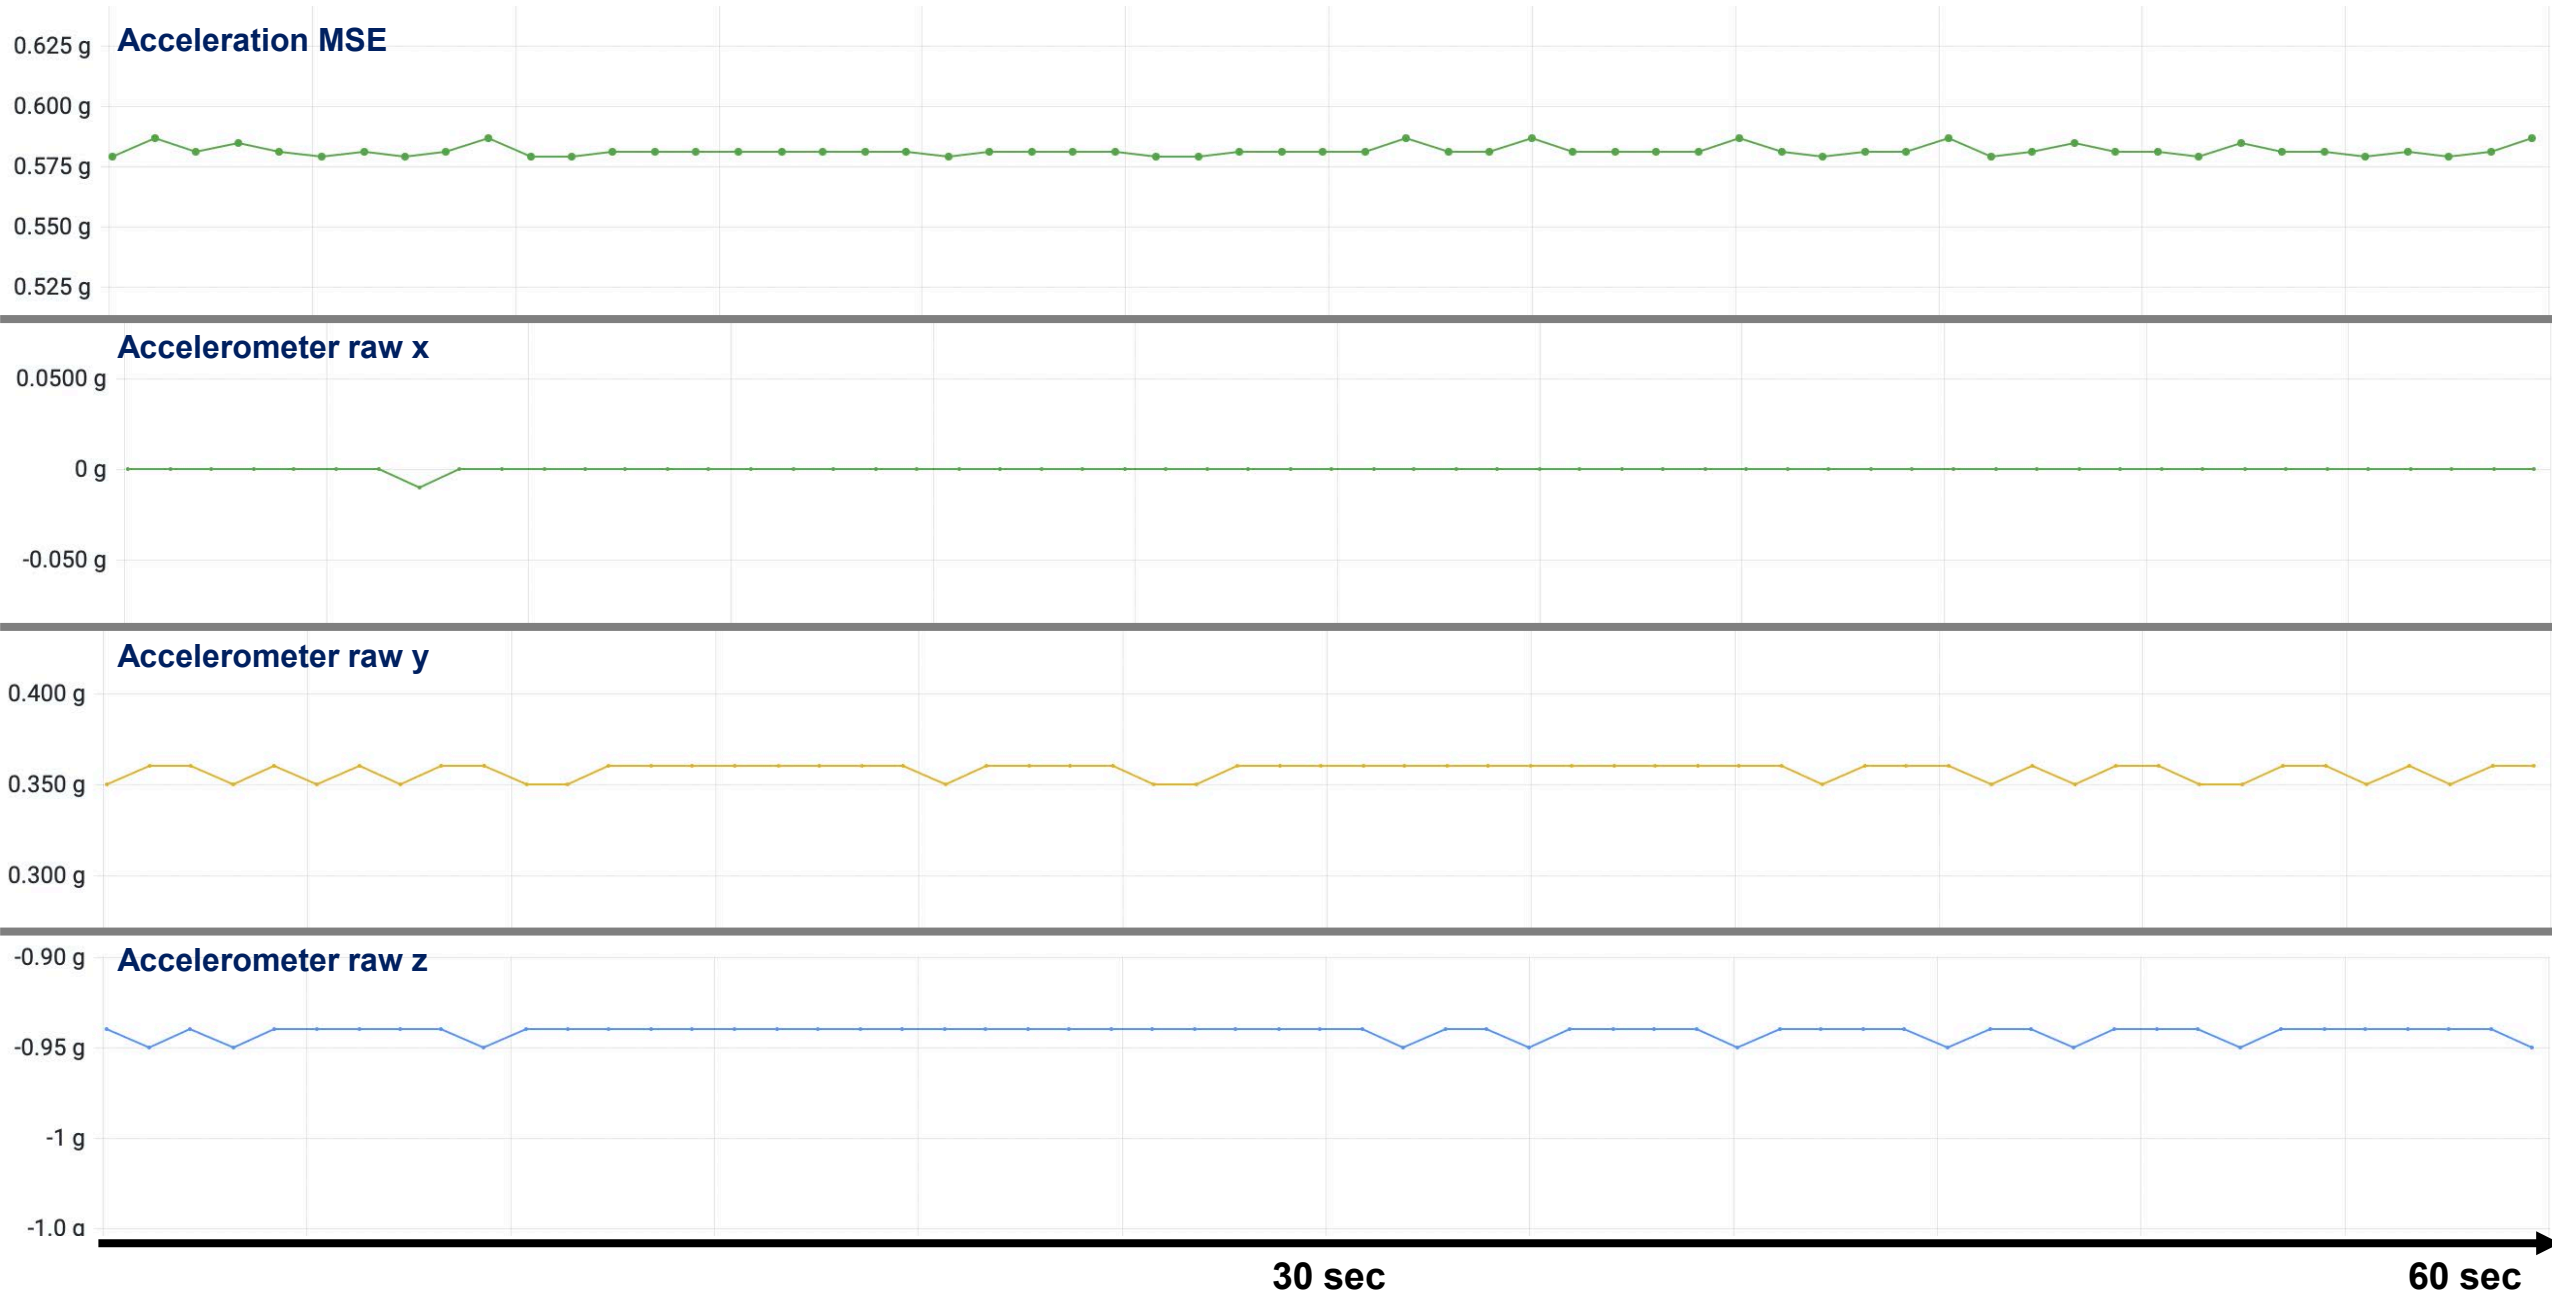


Scene 5: Subject lying in bed motionless, breathing shallow. Panel classification: Scene 20. Subject in bed, lying relaxed

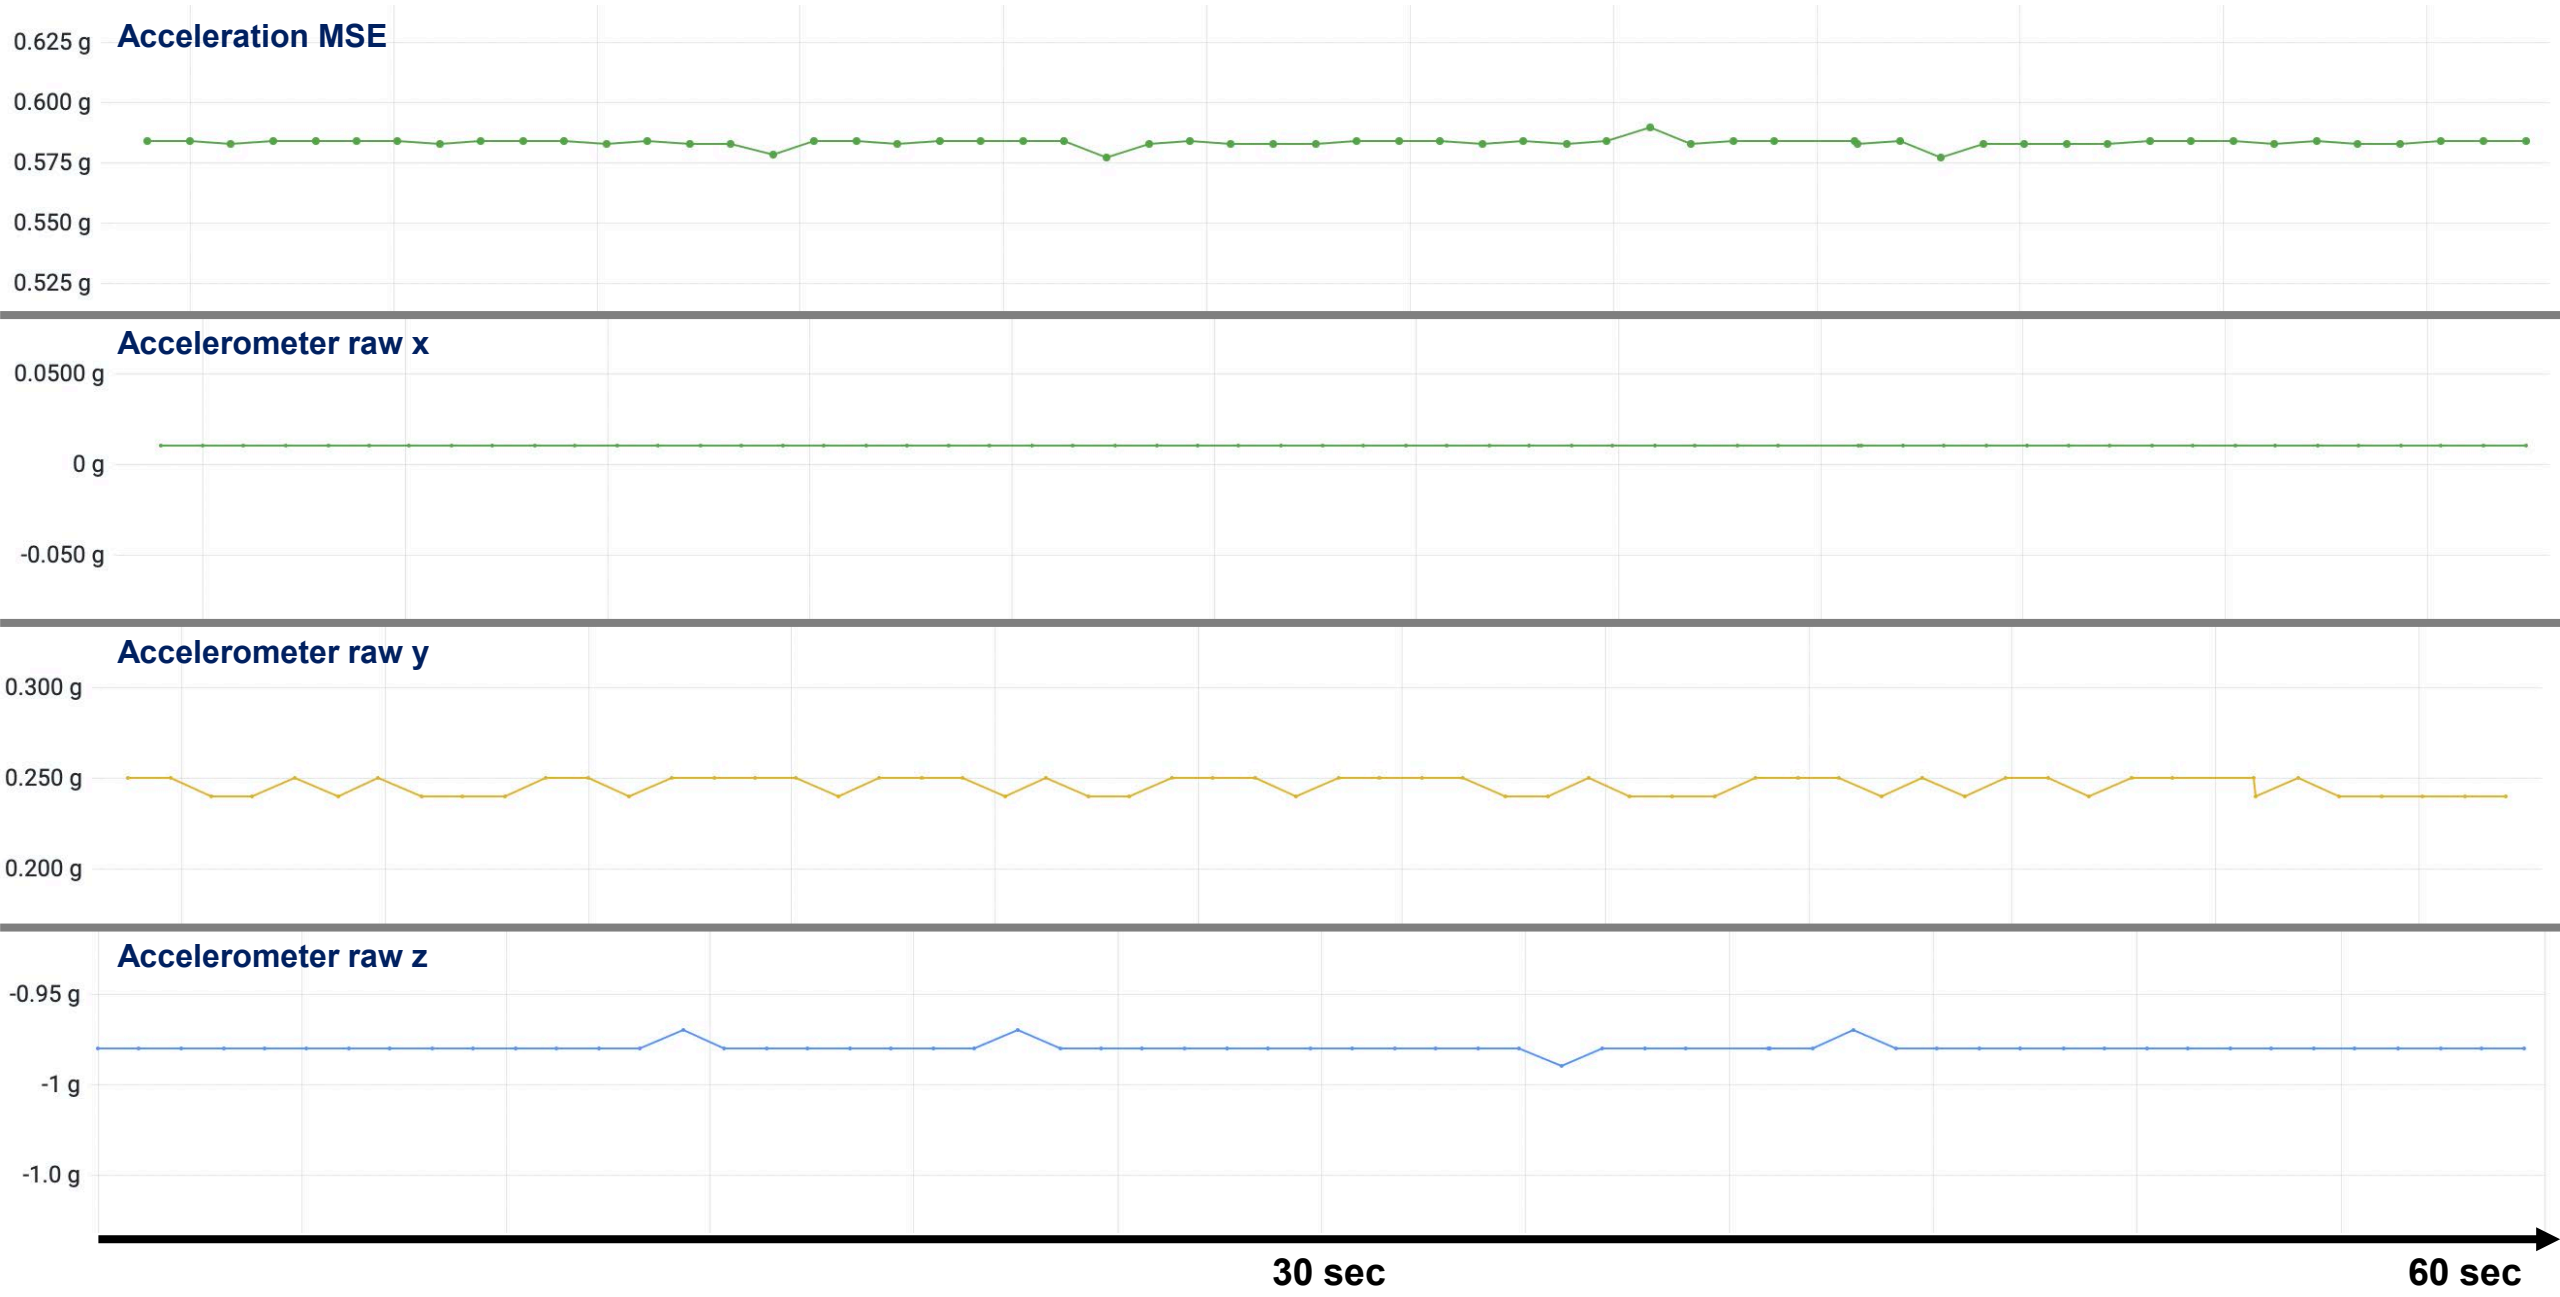


Scene 21: Subject lying in bed motionless, vibrating mobile phone. Panel classification: Scene 20. Subject in bed, lying relaxed

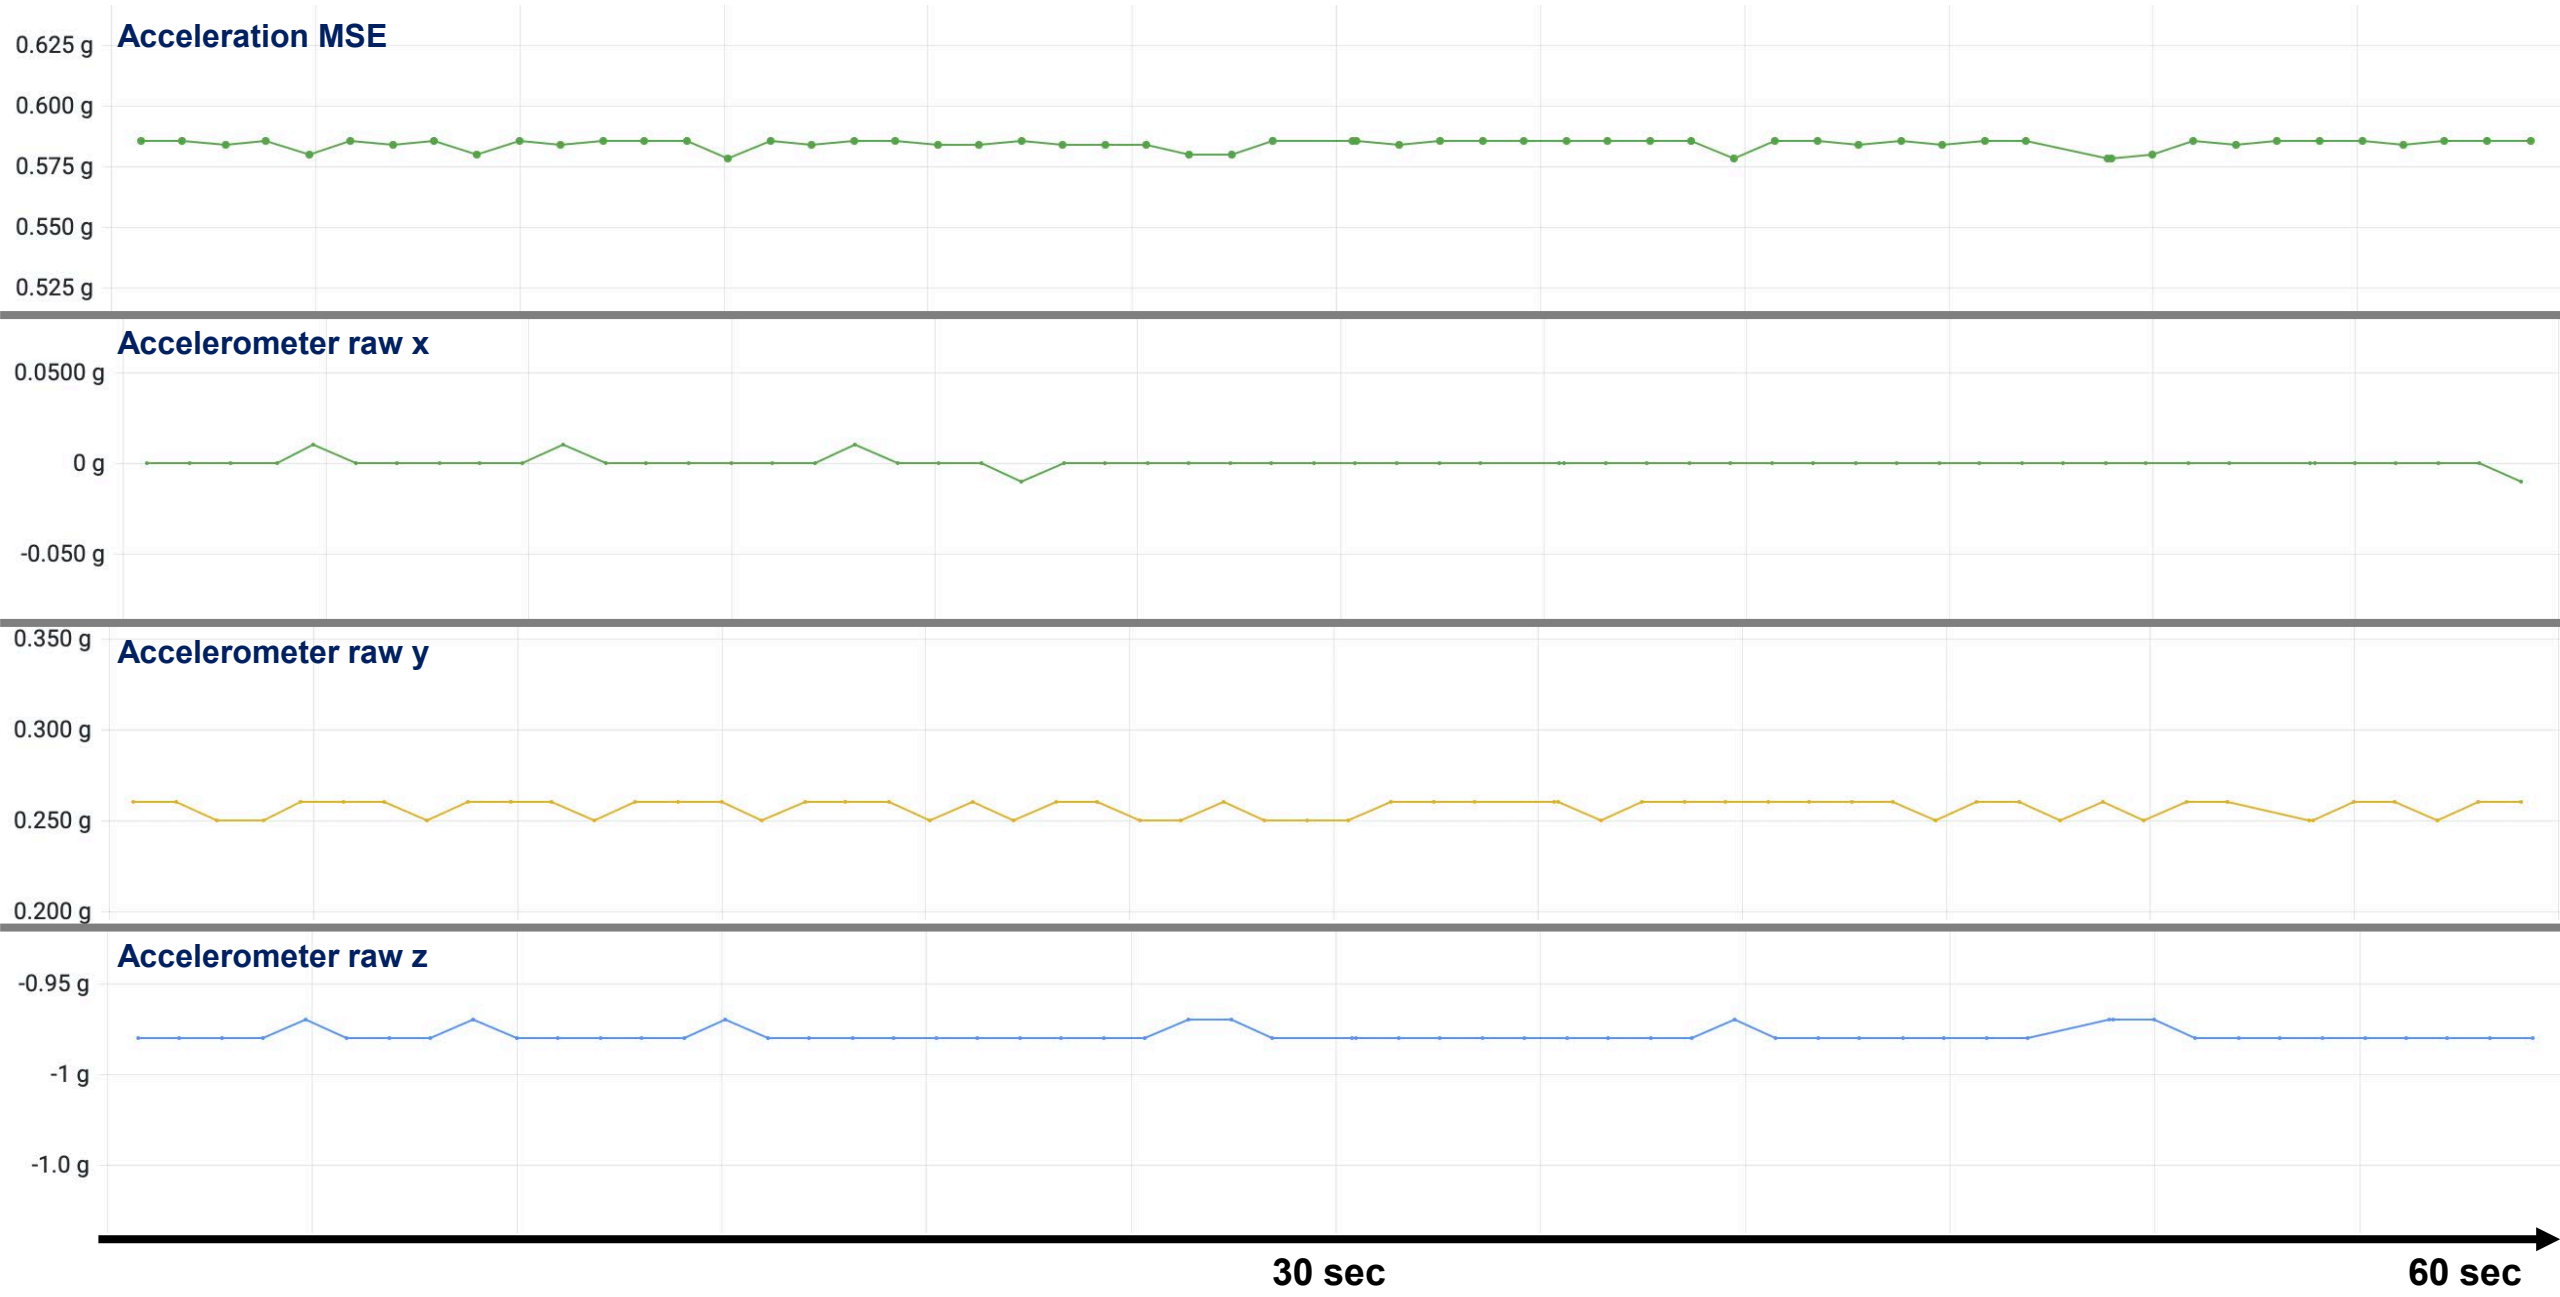

Scene 18: Subject in bed, exhibiting tremor. **Panel classification:** Scene 1. Bed empty

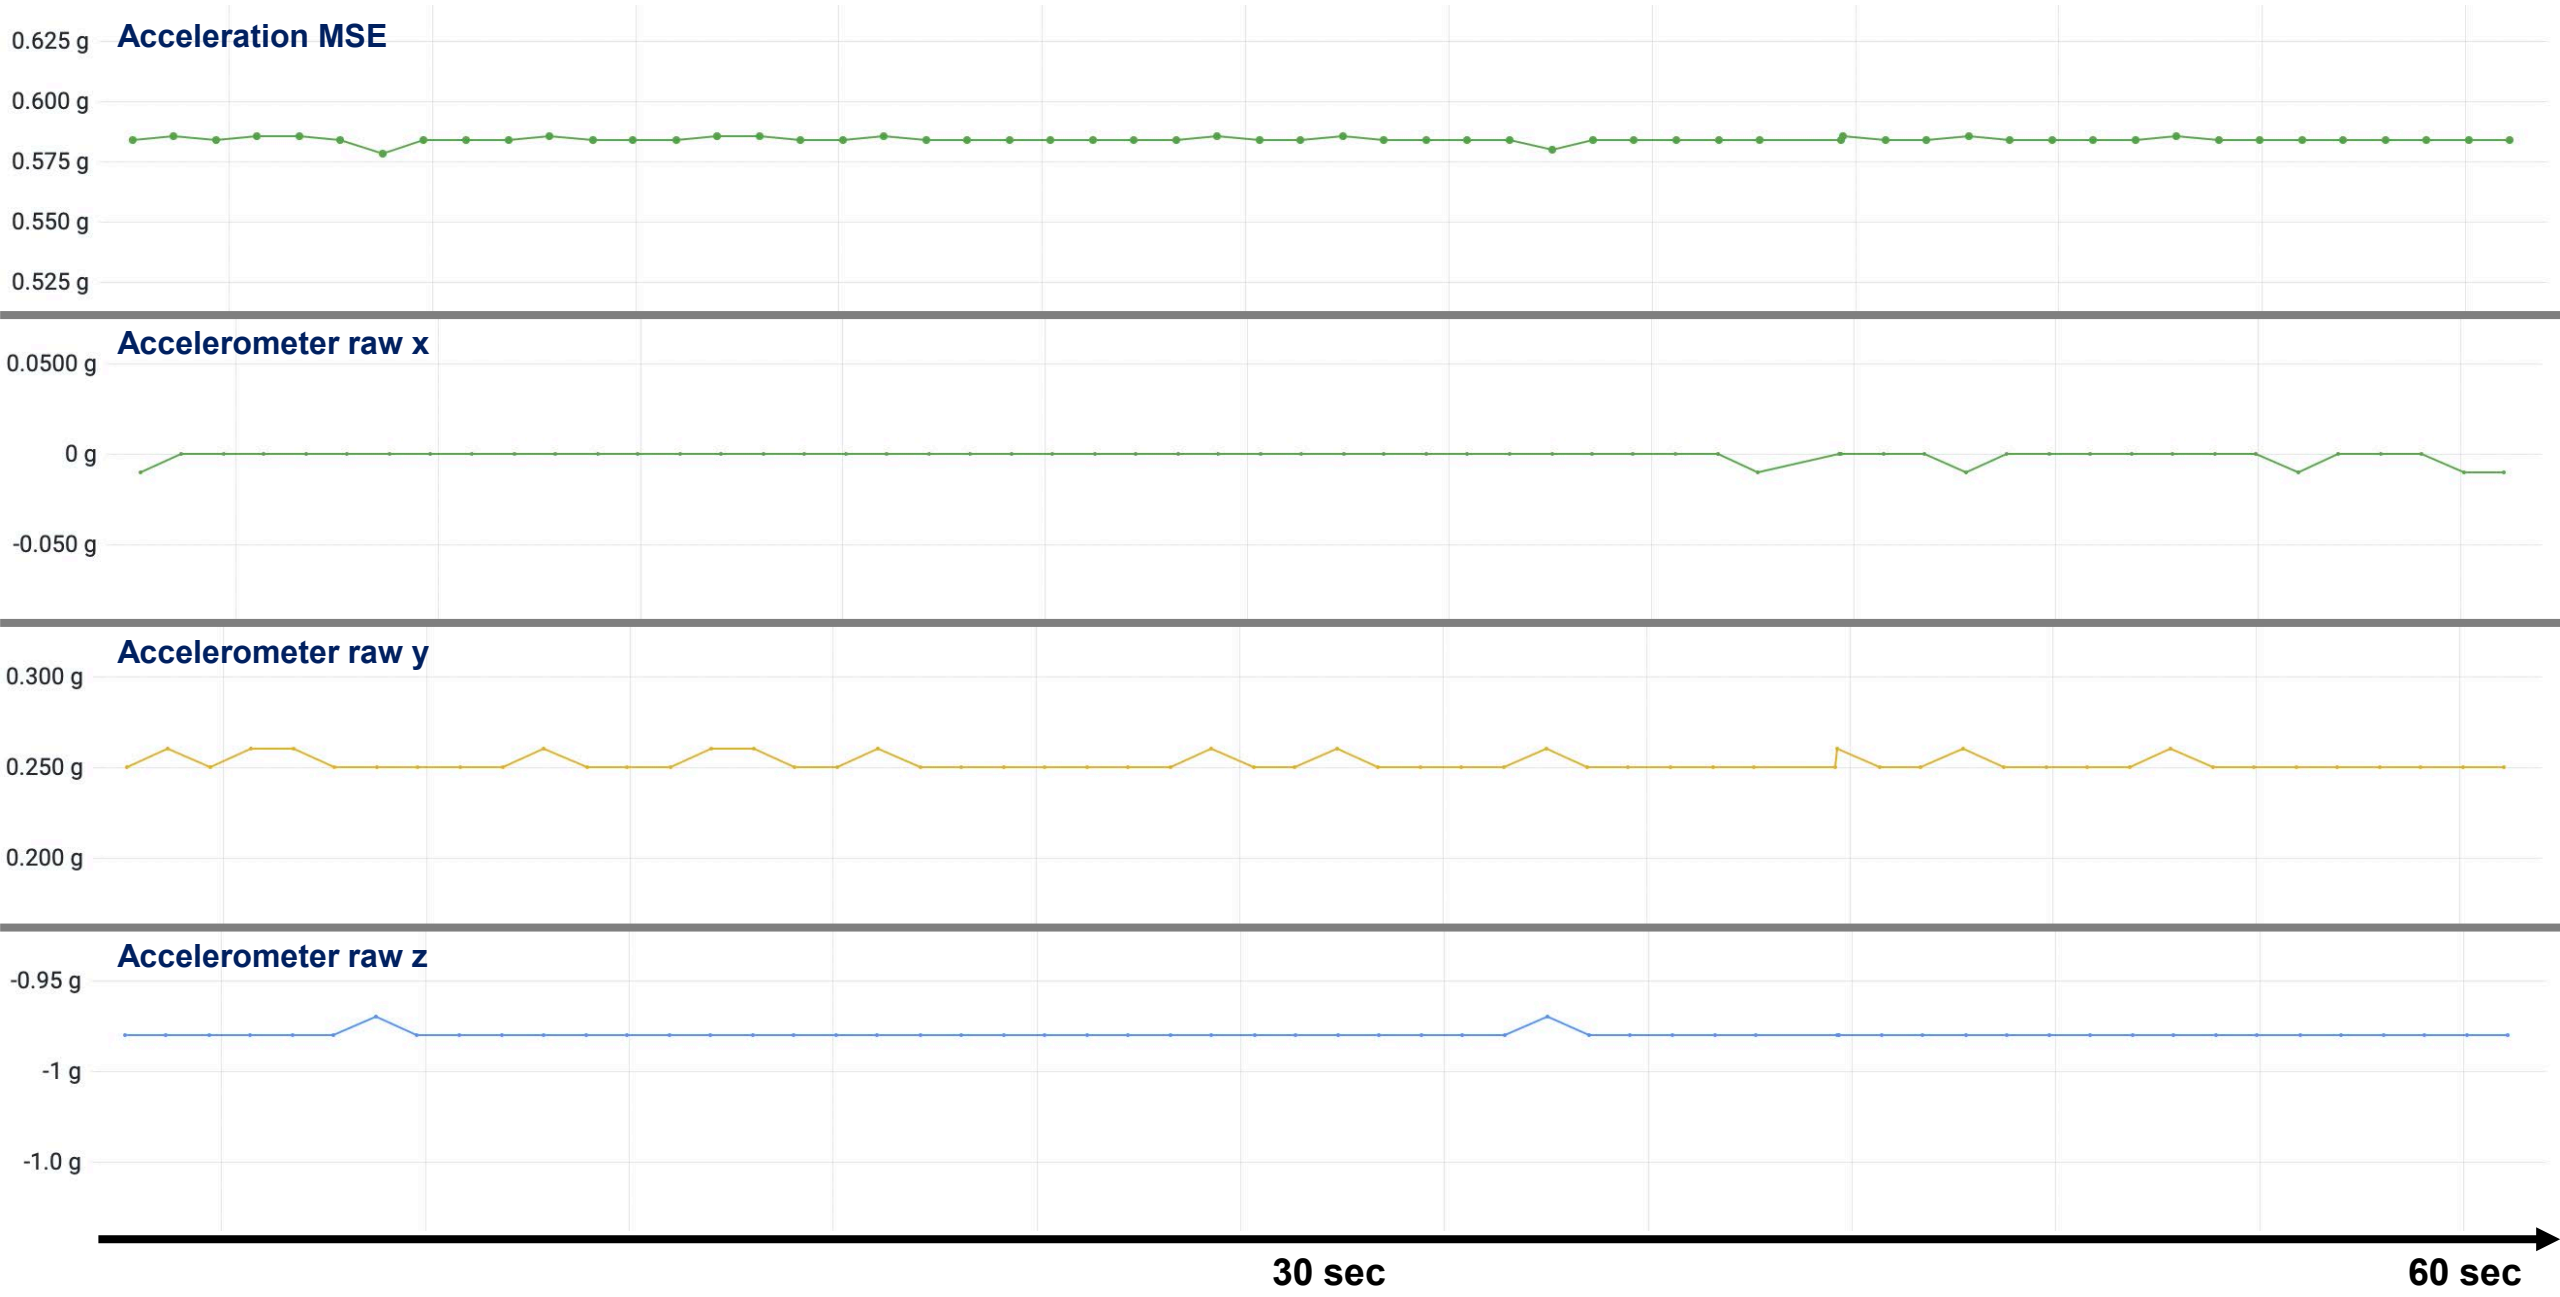

Scene 2: Subject in bed, wires being attached for standard monitoring . Panel classification: Scene 1. Bed empty

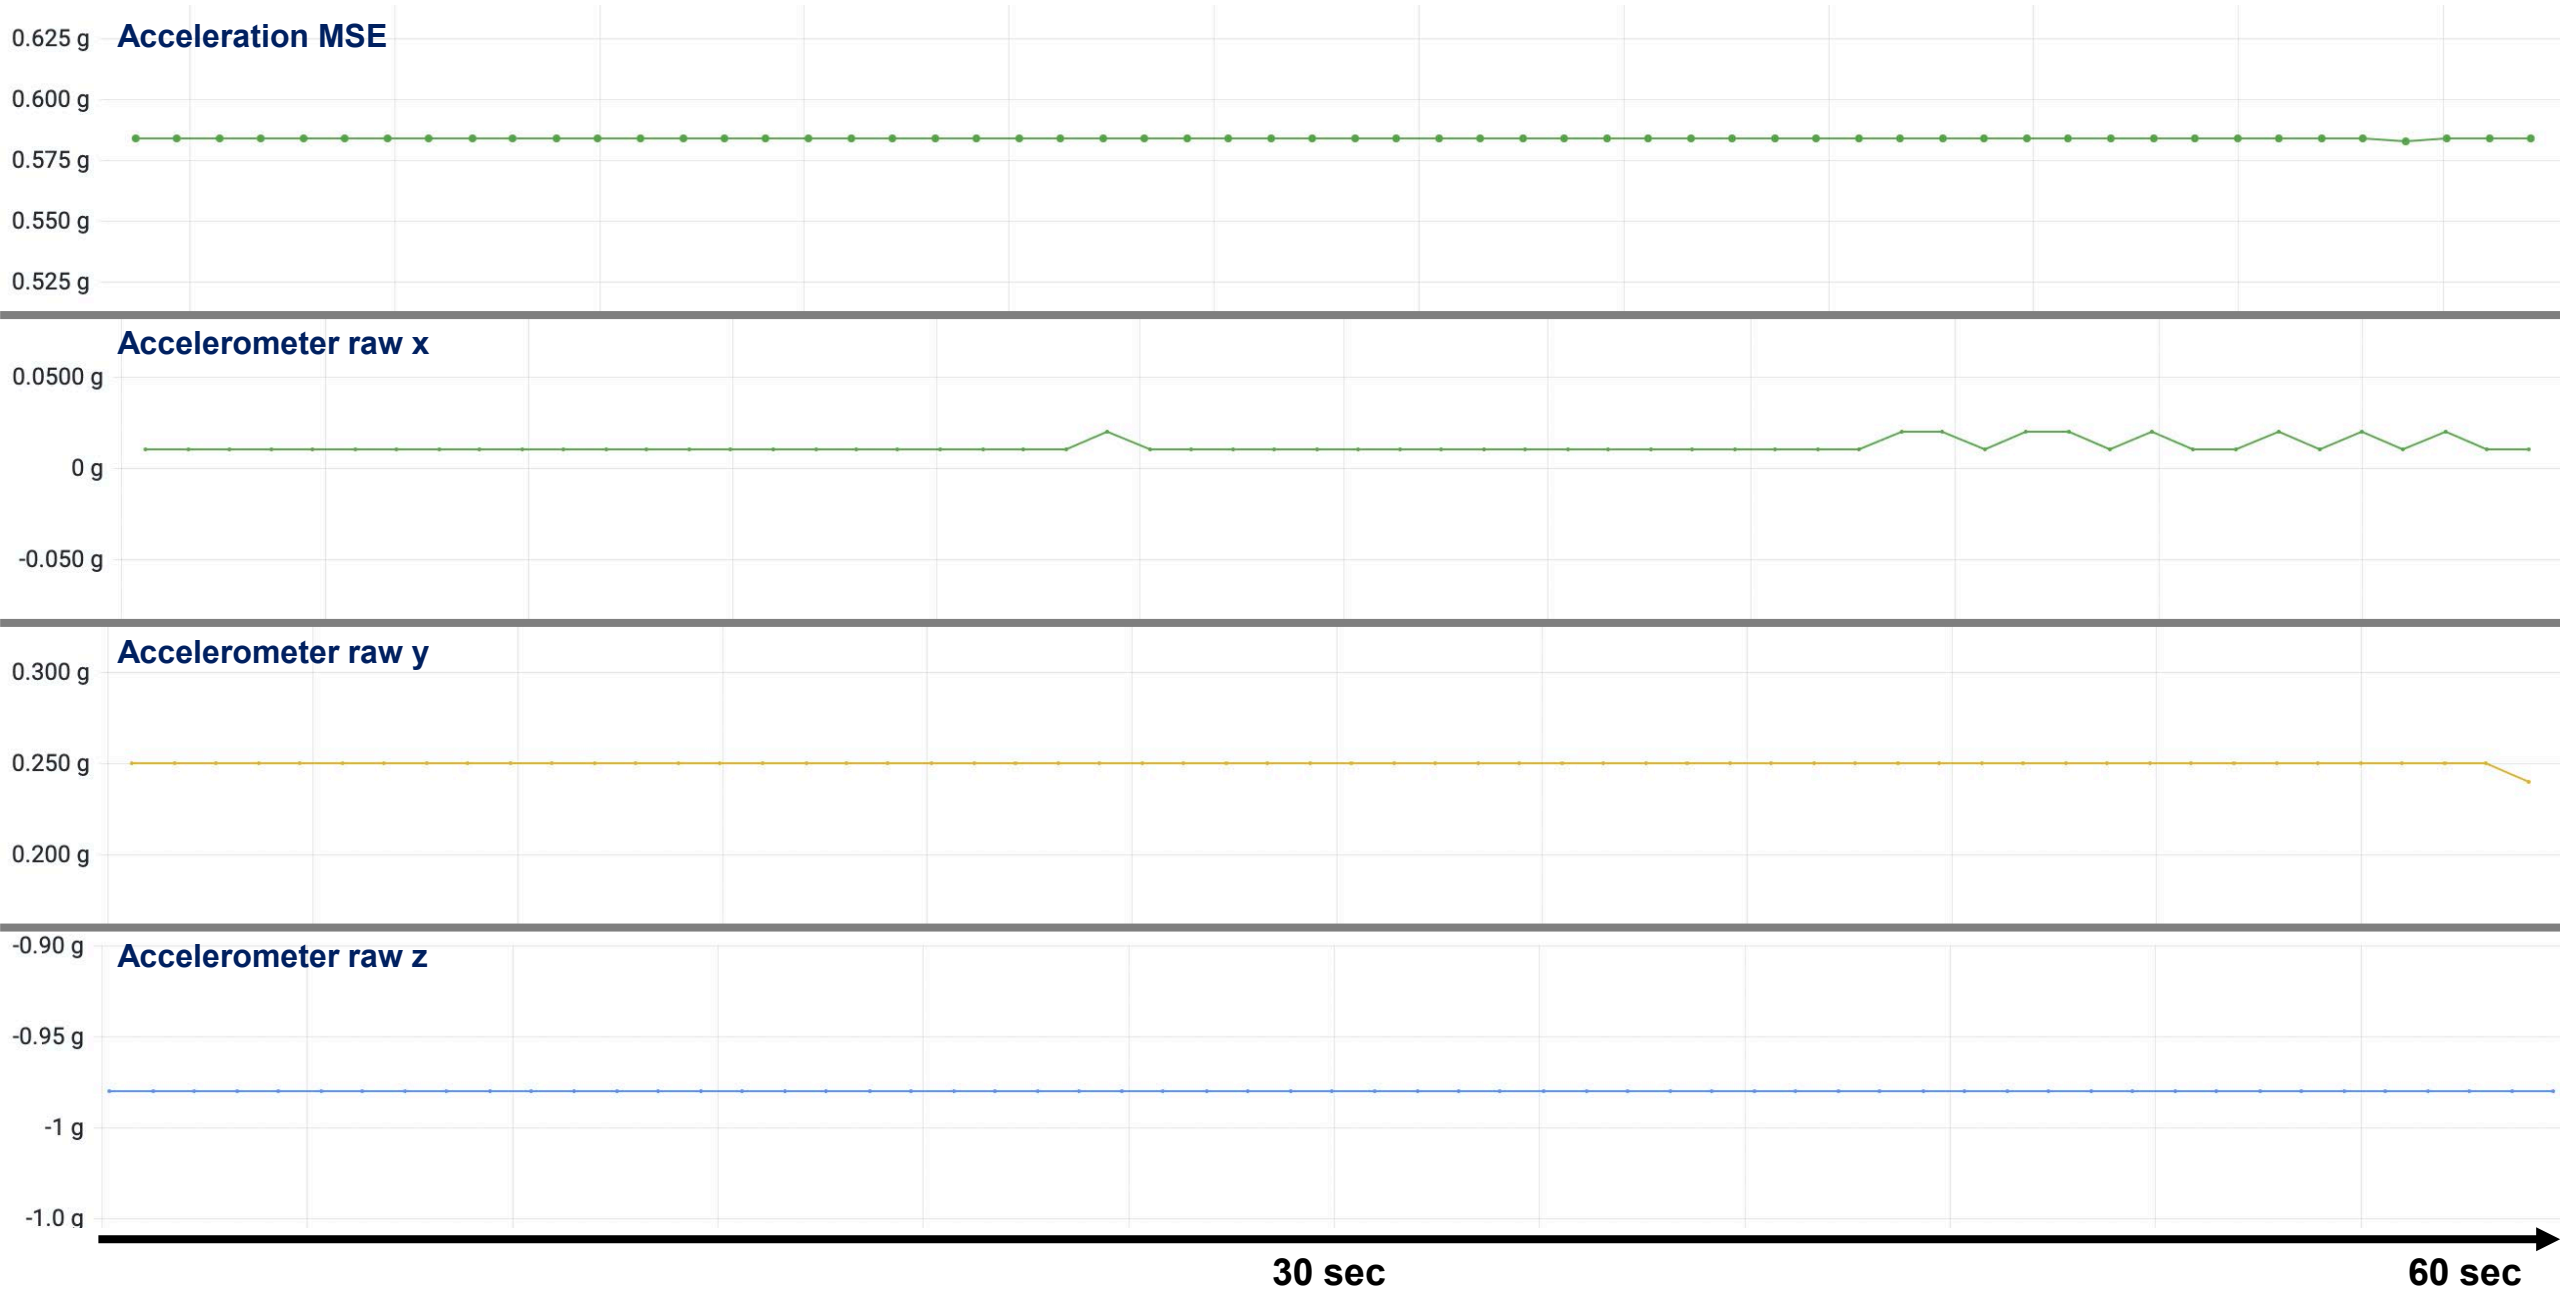

Scene 20: Subject in bed, lying relaxed. Panel classification: Scene 1. Bed empty

