

Supporting Information for

Mesoporous silica-gold films for straightforward, highly reproducible monitoring of mercury traces in water

Anna Mutschler, Vivian Stock, Lena Ebert, Emma Björk, Kerstin Leopold* and Mika Lindén*

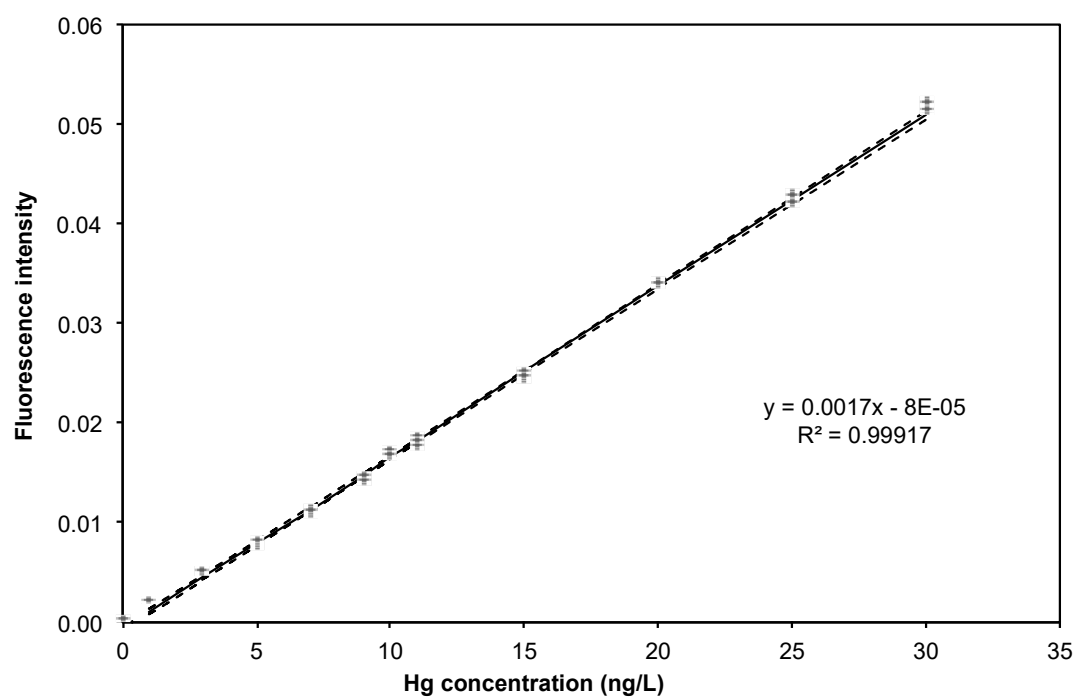


Figure S1. Calibration curve for CV-AFS measurement of Hg in a concentration range from 1 to 30 ng Hg L⁻¹ with a sample volume of 2.2 mL corresponding to absolute Hg masses of 2.09 pg to 62.70 pg.