

Supplementary Materials: Evaluation of Passivation Process for Stainless Steel Hypotubes Used in Coronary Angioplasty Technique

Lucien Reclaru ^{1,2} and Lavinia Cosmina Ardelean ^{2,3,*}

¹ Scientific Independent Consultant Biomaterials and Medical Devices, 103 Paul-Vouga, 2074 Marin-Neuchâtel, Switzerland; lreclaru@gmail.com

² Multidisciplinary Center for Research, Evaluation, Diagnosis and Therapies in Oral Medicine, "Victor Babes" University of Medicine and Pharmacy Timisoara, 2 Eftimie Murgu sq, 300041 Timisoara, Romania

³ Department of Technology of Materials and Devices in Dental Medicine, "Victor Babes" University of Medicine and Pharmacy Timisoara, 2 Eftimie Murgu sq, 300041 Timisoara, Romania

* Correspondence: lavinia_ardelean@umft.ro

Citation: Reclaru, L.; Ardelean, L.C.; Evaluation of Passivation Process for Stainless Steel Hypotubes Used in Coronary Angioplasty Technique. *Coatings* **2021**, *11*, 448. <https://doi.org/10.3390/coatings11040448>

Academic Editor: Antonella Rossi

Received: 17 March 2021

Accepted: 10 April 2021

Published: 13 April 2021

Publisher's Note: MDPI stays neutral with regard to jurisdictional claims in published maps and institutional affiliations.



Copyright: © 2021 by the authors. Submitted for possible open access publication under the terms and conditions of the Creative Commons Attribution (CC BY) license (<http://creativecommons.org/licenses/by/4.0/>).

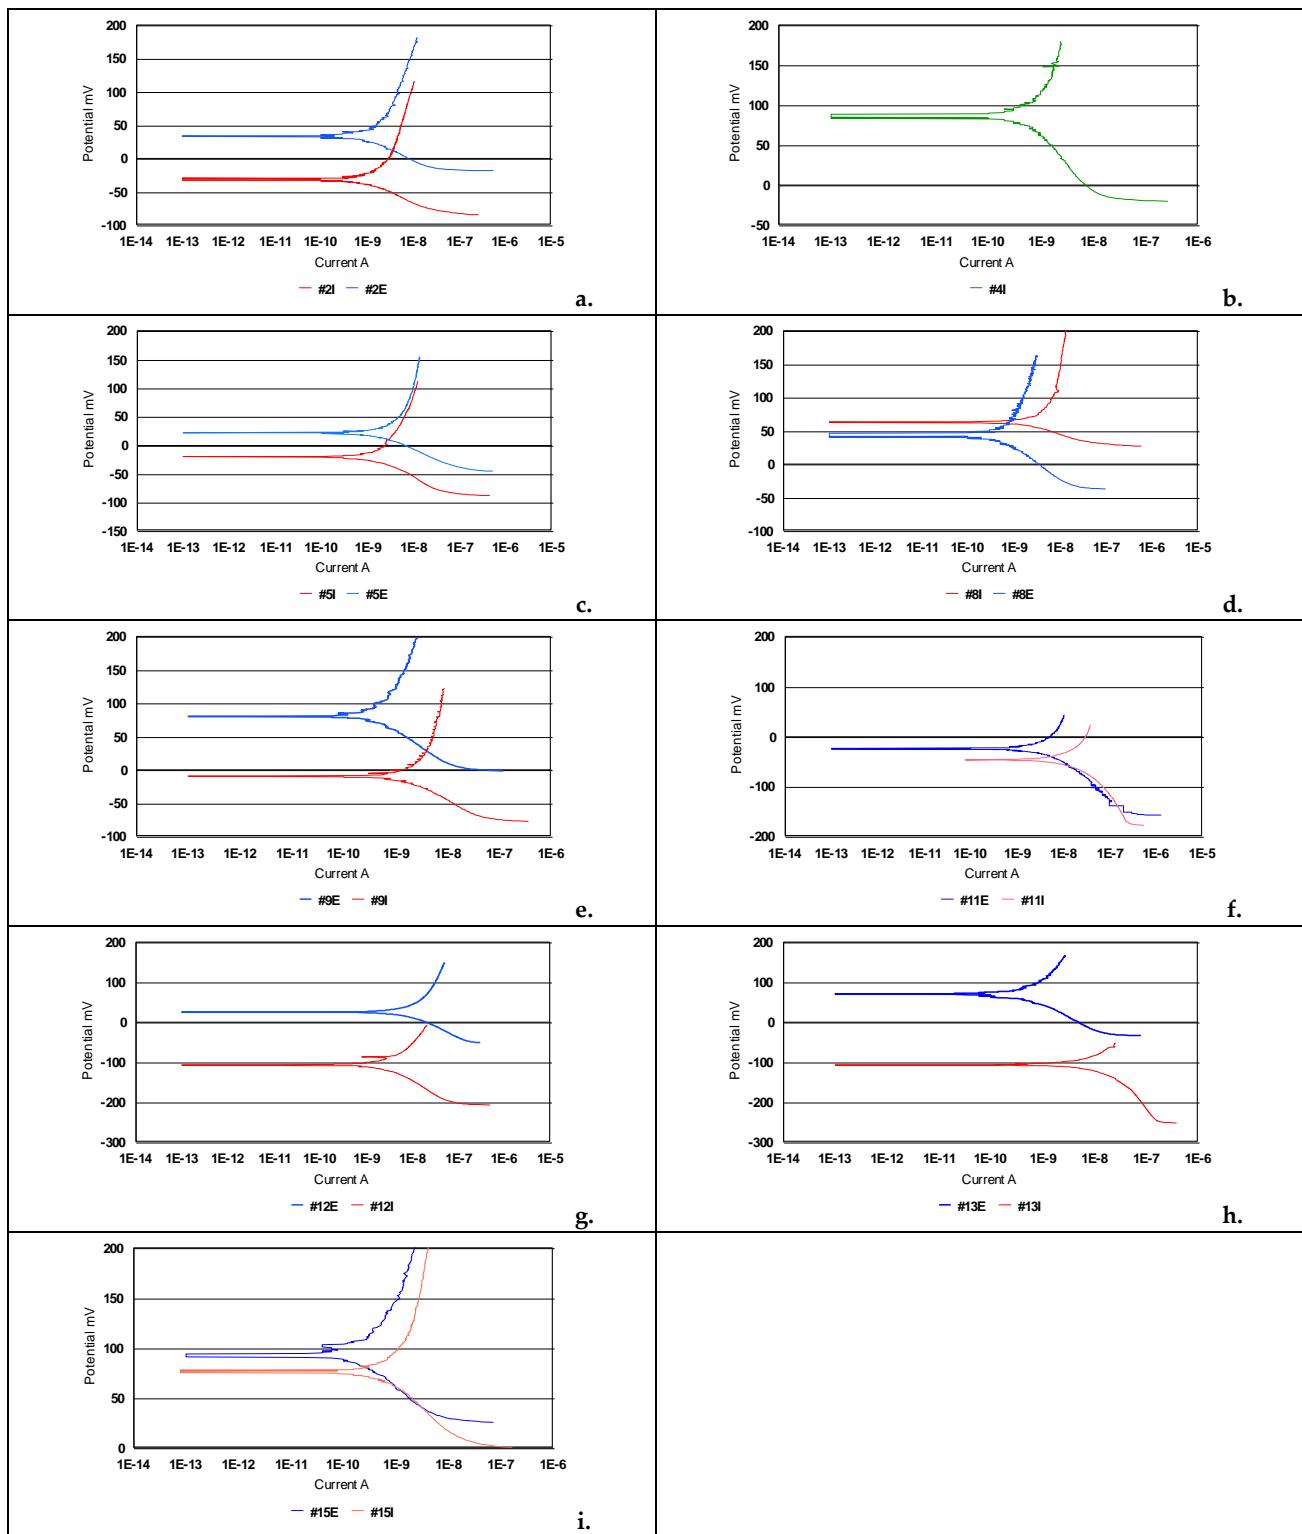


Figure S1. Polarization curves in the Tafel domain of the hypotubes: (a). #2(ref), (b). #4, (c). #5, (d). #8(ref), (e). #9, (f). #11, (g). #12, (h). #13(ref), (i). #15. E: external surface; I: internal surface.